
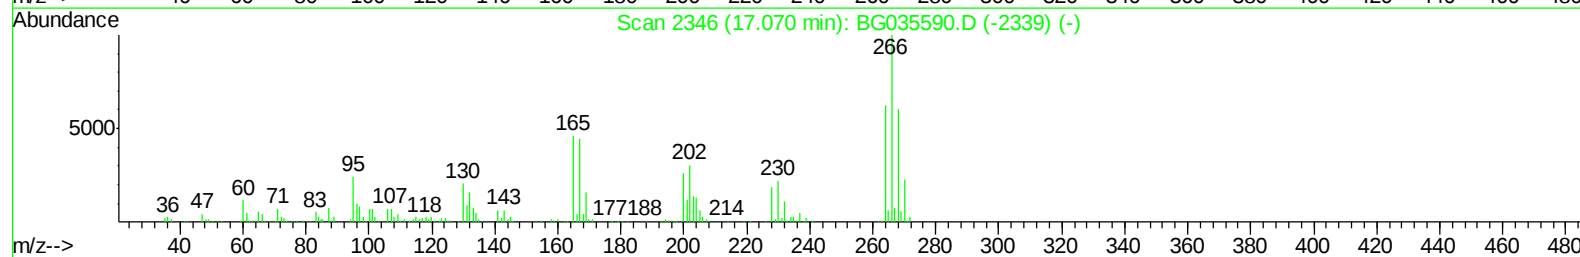
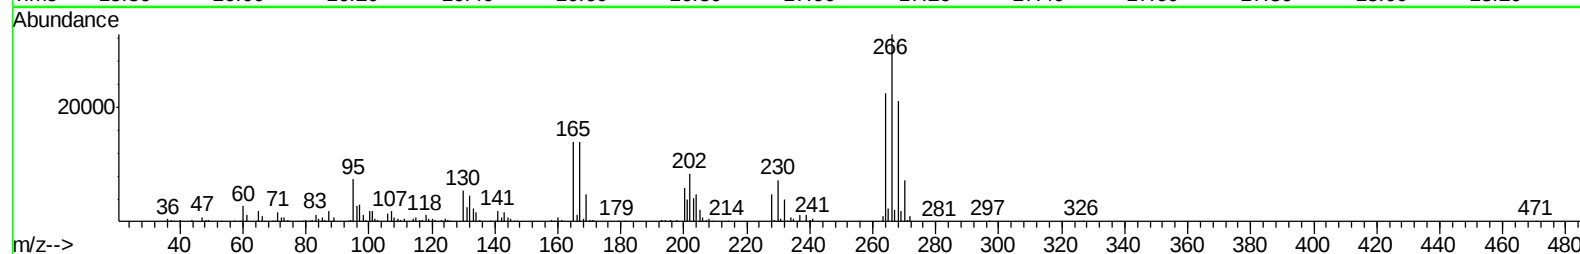


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data File : BG035699.D
Acq On : 18 Jul 2018 2:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 06:36:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

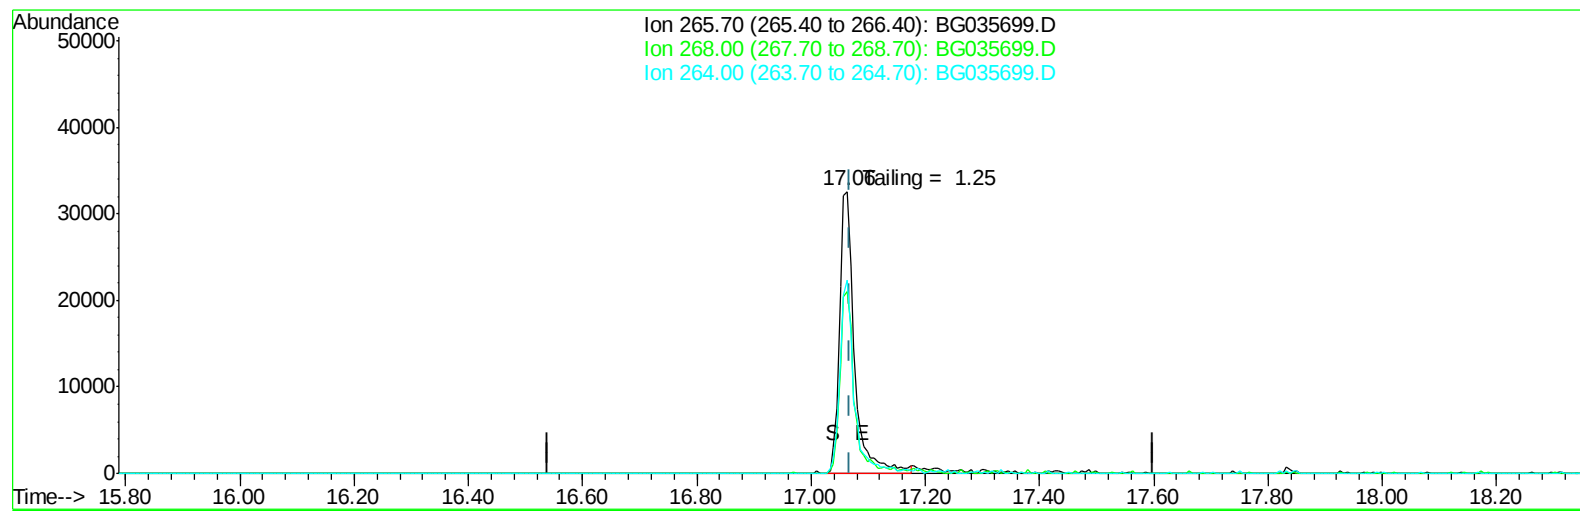

TIC: BG035699.D

(69) Pentachlorophenol (C)




17.063min (-0.007) 1456.96ng

response 58696

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.41
264.00	62.00	68.78
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data File : BG035699.D
Acq On : 18 Jul 2018 2:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 06:36:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

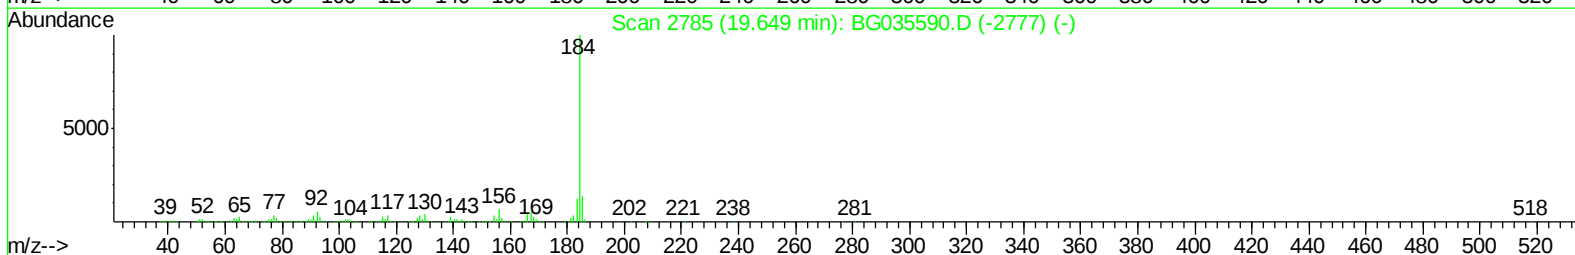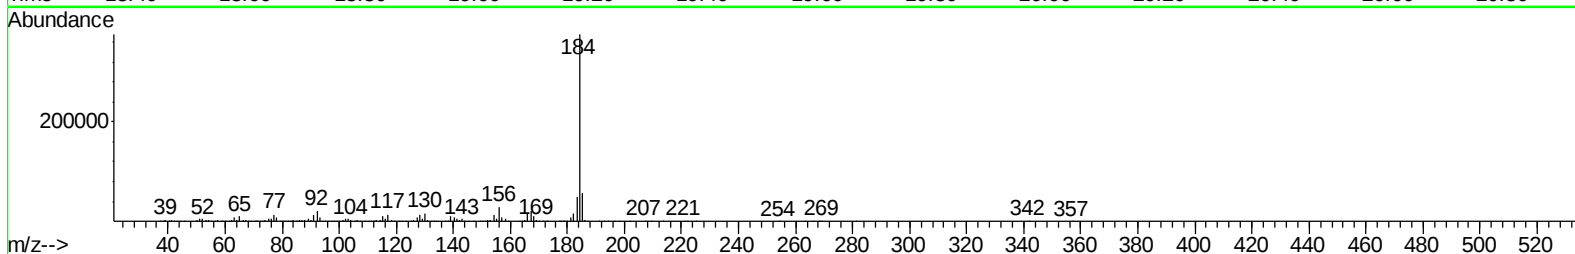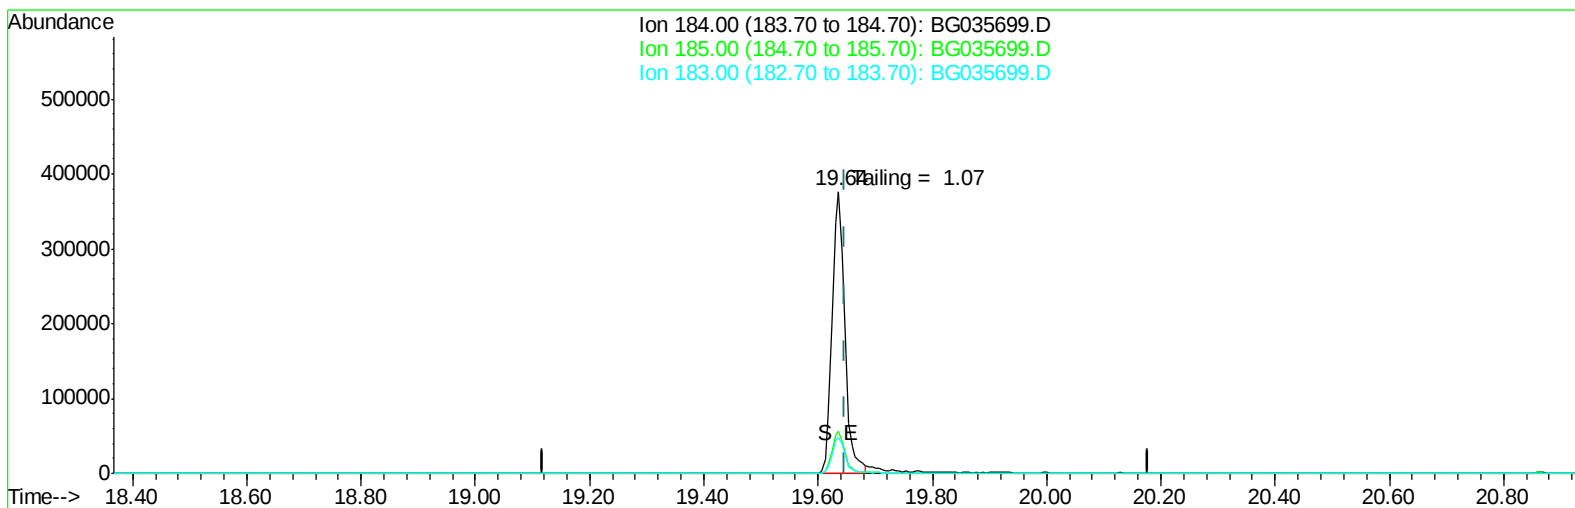

TIC: BG035699.D

(76) Benzidine

19.636min (-0.013) 4079.12ng

response 588325

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.16
183.00	13.30	12.83
0.00	0.00	0.00