

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
 Data File : BG035701.D
 Acq On : 18 Jul 2018 3:49
 Operator : JU/SJ
 Sample : J3990-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 071218-DBRI-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.625	391	398	412	rBV	324183	557795	11.52%	2.929%
2	7.205	657	667	680	rBV	224139	432008	8.92%	2.269%
3	7.576	722	730	743	rBV	614404	1028347	21.23%	5.400%
4	8.040	802	809	817	rBV	186341	324112	6.69%	1.702%
5	8.363	856	864	875	rVB	801651	1399985	28.90%	7.351%
6	9.203	999	1007	1018	rBV	653620	1210265	24.98%	6.355%
7	10.842	1278	1286	1297	rBV	221910	417798	8.63%	2.194%
8	13.285	1695	1702	1716	rBV	1847311	2899050	59.85%	15.223%
9	14.114	1838	1843	1853	rBV	64002	111206	2.30%	0.584%
10	14.660	1930	1936	1946	rBV2	388858	649044	13.40%	3.408%
11	15.947	2151	2155	2166	rBV	69794	96574	1.99%	0.507%
12	16.146	2182	2189	2206	rBV	1011096	1625557	33.56%	8.536%
13	17.403	2396	2403	2413	rBV2	548135	893461	18.44%	4.692%
14	20.012	2841	2847	2853	rBV	3617957	4844006	100.00%	25.436%
15	21.310	3063	3068	3075	rBV6	48671	92788	1.92%	0.487%
16	21.668	3122	3129	3138	rBV2	659441	1097397	22.65%	5.763%
17	23.149	3376	3381	3388	rVB2	35572	64893	1.34%	0.341%
18	23.947	3512	3517	3525	rVB4	39726	77691	1.60%	0.408%
19	24.881	3665	3676	3688	rBV	401844	1127340	23.27%	5.920%
20	26.009	3861	3868	3878	rVB8	30122	94406	1.95%	0.496%


Sum of corrected areas: 19043723

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
Data File : BG035701.D
Acq On : 18 Jul 2018 3:49
Operator : JU/SJ
Sample : J3990-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

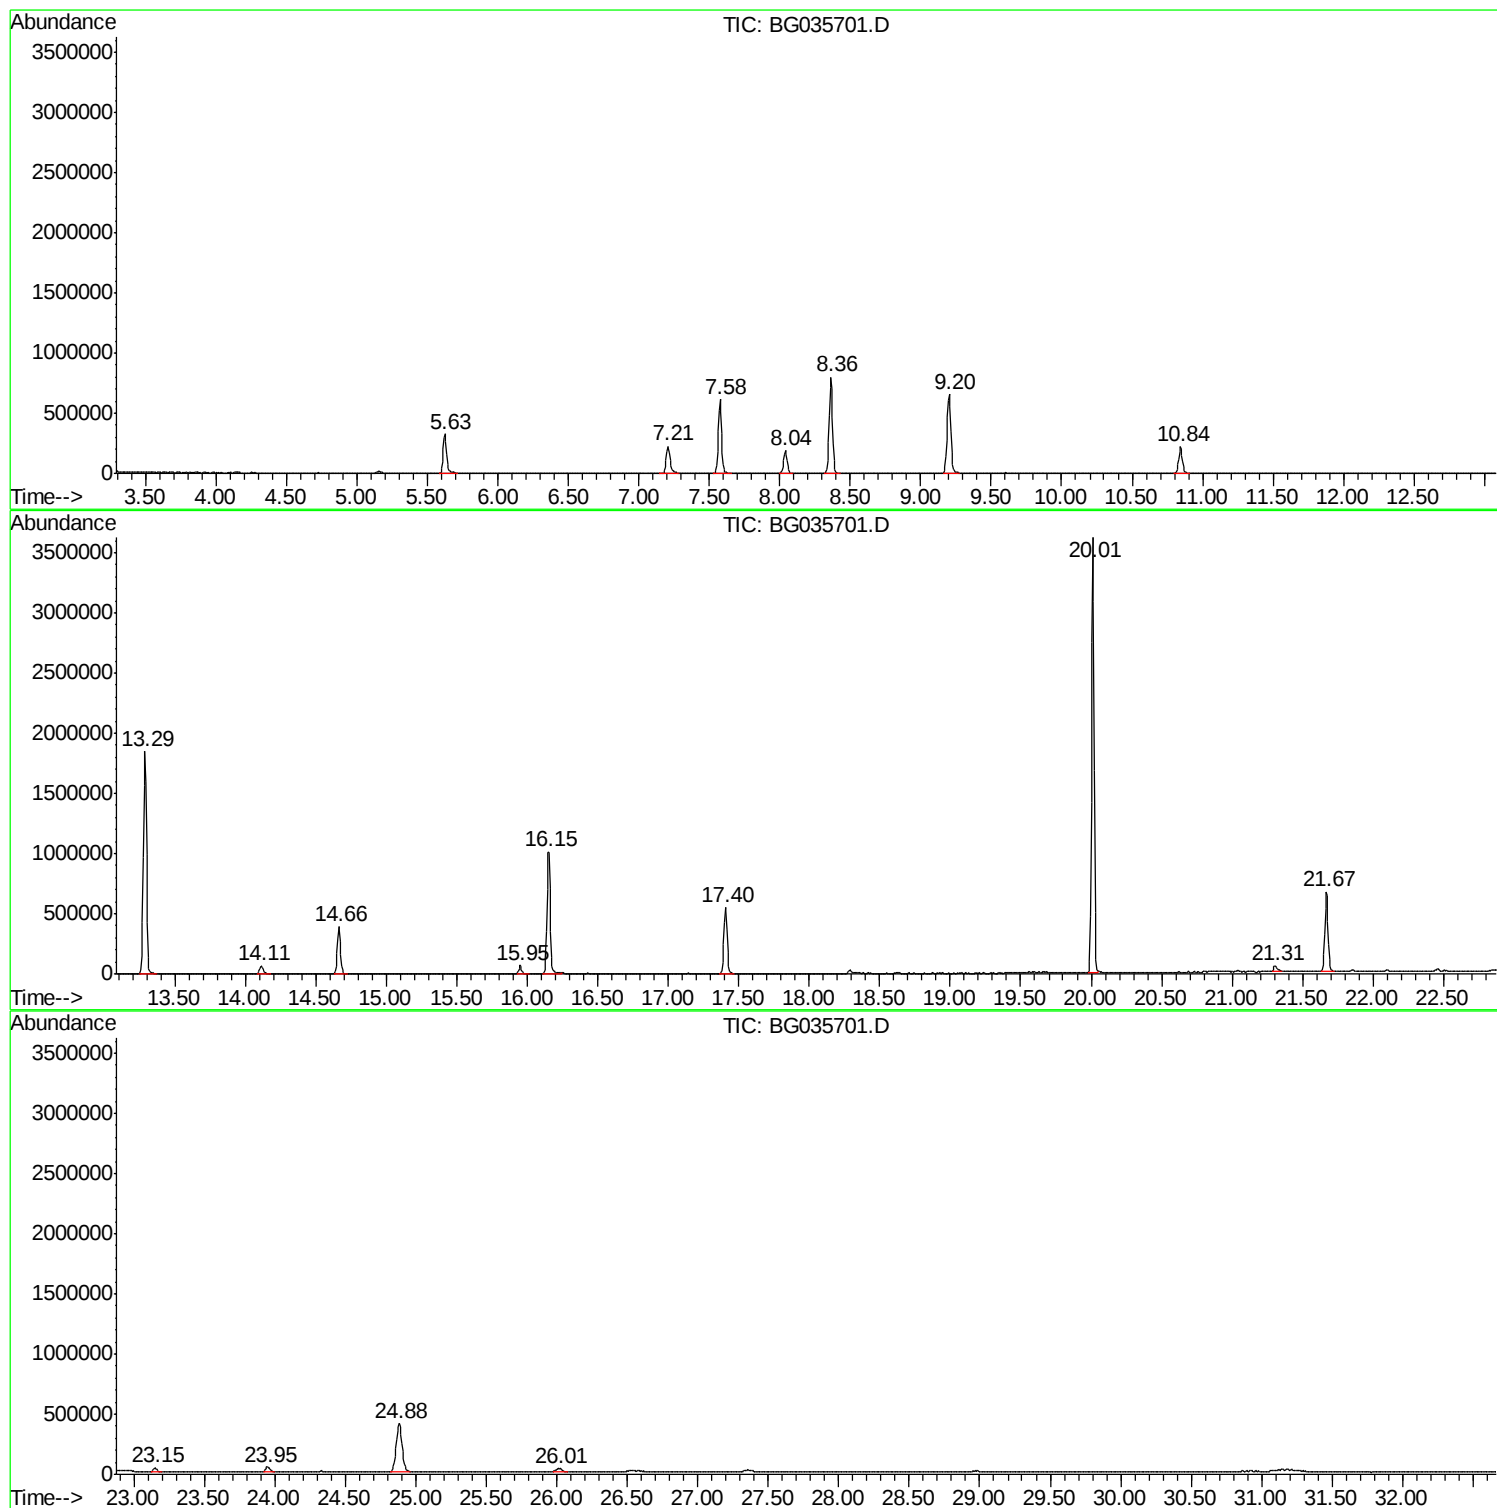

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data_File : BG035701.D
Acq_On : 18-Jul-2018 3:499
Operator : JU/SJJ
Sample : J3990-011
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
