

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
 Data File : BG035705.D
 Acq On : 18 Jul 2018 6:25
 Operator : JU/SJ
 Sample : J3990-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 071218-DBRI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.621	390	397	411	rBV	327817	556696	12.57%	3.140%
2	7.207	660	667	682	rBV	233505	460907	10.41%	2.600%
3	7.577	722	730	746	rVB	565499	973775	21.99%	5.493%
4	8.041	802	809	817	rBV	180847	302464	6.83%	1.706%
5	8.364	856	864	874	rBV	733145	1287337	29.07%	7.261%
6	9.204	995	1007	1019	rBV	586224	1087631	24.56%	6.135%
7	10.843	1279	1286	1298	rBV	192300	367486	8.30%	2.073%
8	13.287	1695	1702	1714	rBV	1708777	2630791	59.42%	14.839%
9	14.109	1836	1842	1852	rBV	113803	188846	4.27%	1.065%
10	14.661	1929	1936	1945	rBV2	356830	580708	13.12%	3.276%
11	15.948	2149	2155	2162	rBV	35708	47752	1.08%	0.269%
12	16.148	2181	2189	2207	rBV	961955	1483445	33.50%	8.368%
13	17.405	2397	2403	2410	rBV	525360	818367	18.48%	4.616%
14	20.013	2841	2847	2856	rBV	3361963	4427783	100.00%	24.975%
15	21.305	3062	3067	3076	rBV2	74772	124982	2.82%	0.705%
16	21.669	3122	3129	3139	rBV2	606363	992173	22.41%	5.596%
17	22.462	3259	3264	3268	rBV2	33147	56116	1.27%	0.317%
18	23.150	3373	3381	3387	rBV3	46389	93462	2.11%	0.527%
19	23.949	3511	3517	3526	rVB2	53825	111312	2.51%	0.628%
20	24.883	3666	3676	3688	rBV	360975	1025642	23.16%	5.785%
21	26.011	3859	3868	3878	rVB5	36366	110914	2.50%	0.626%


Sum of corrected areas: 17728589

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
Data File : BG035705.D
Acq On : 18 Jul 2018 6:25
Operator : JU/SJ
Sample : J3990-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

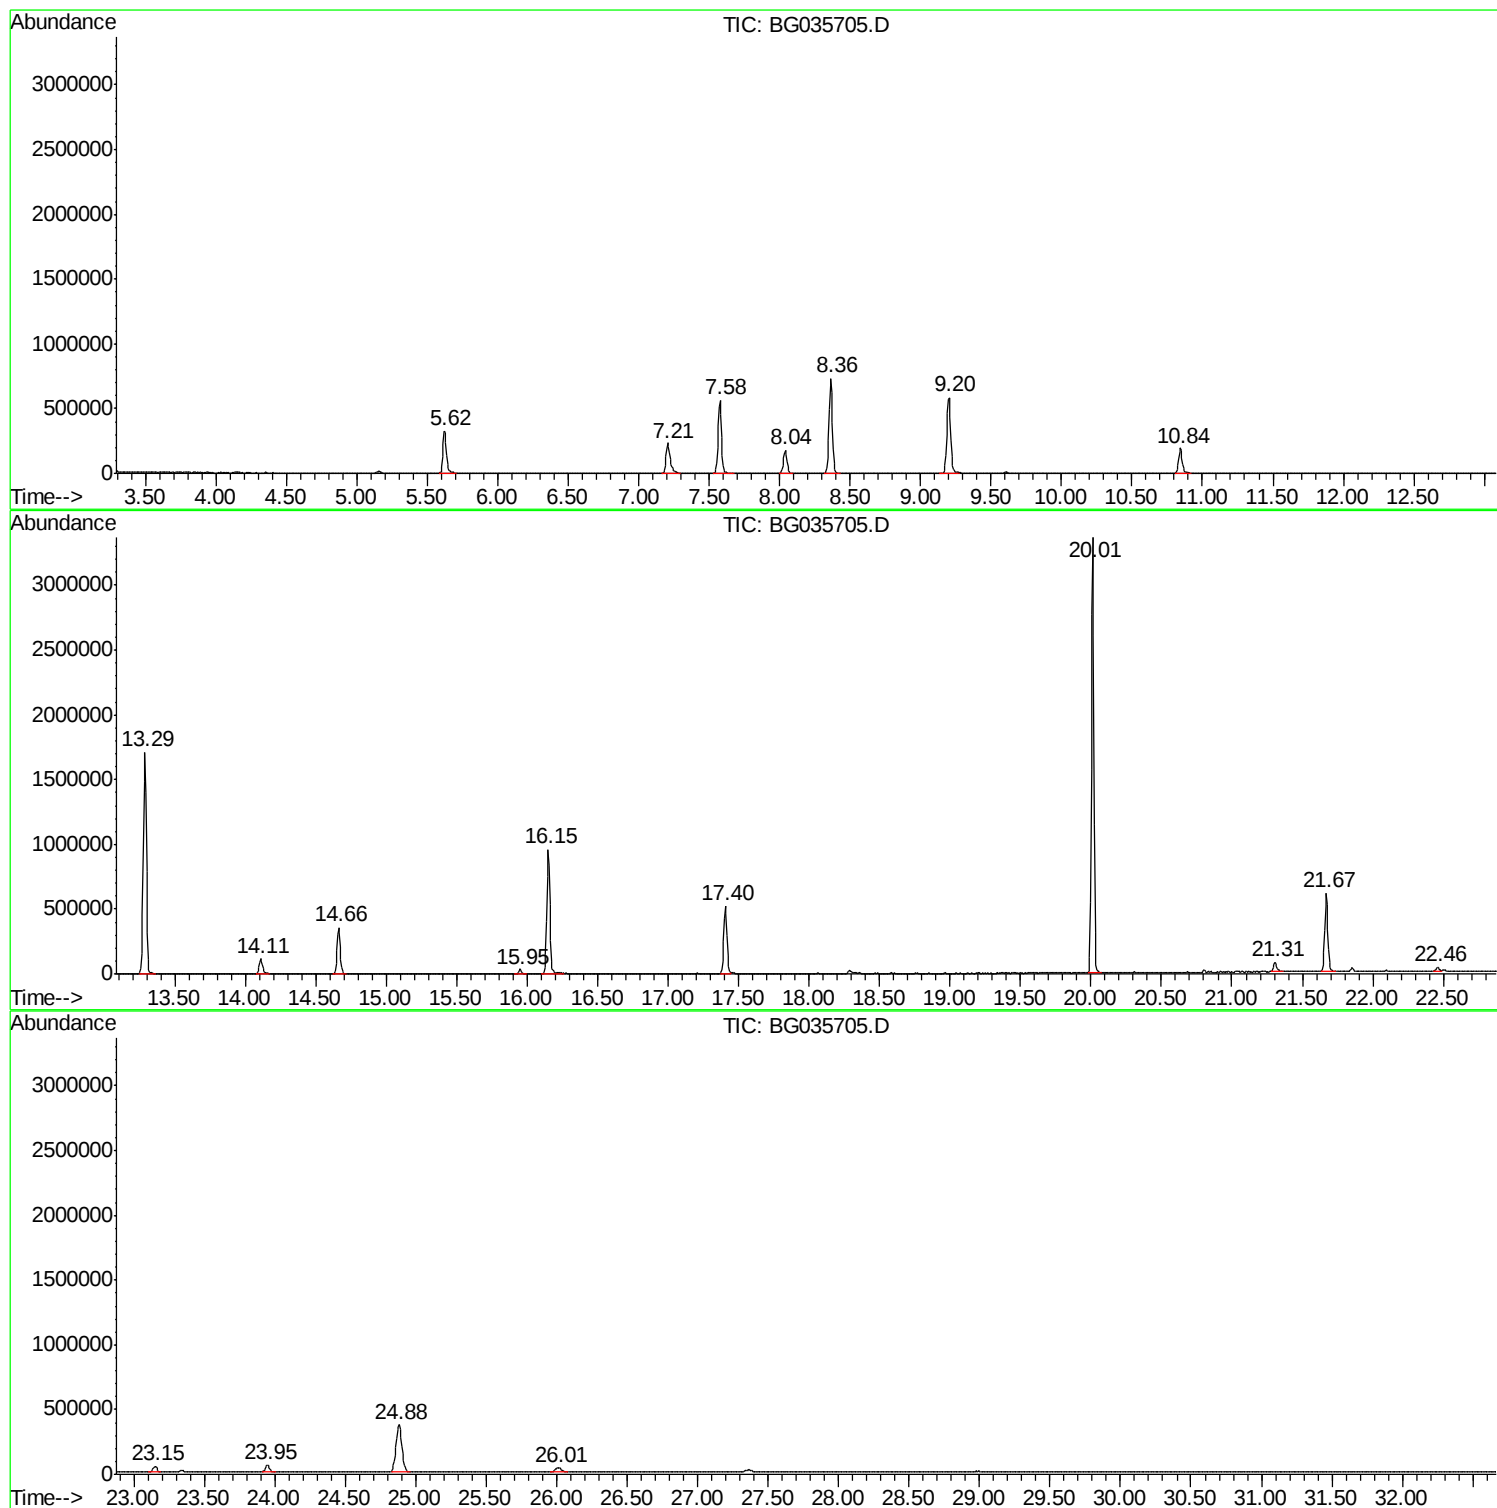

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data_File : BG035705.D
Acq_On : 18-Jul-2018 6:255
Operator : JU/SJJ
Sample : J3990-055
Misc :
ALS_Vial : 24 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-U-M

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
