

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
 Data File : BG035706.D
 Acq On : 18 Jul 2018 7:04
 Operator : JU/SJ
 Sample : J3990-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 071218-DBRI-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.625	389	398	408	rBV	309115	537477	11.30%	2.937%
2	7.206	660	667	683	rBV	223893	447080	9.40%	2.443%
3	7.576	723	730	742	rBV	566608	990658	20.83%	5.412%
4	8.040	802	809	818	rBV	174362	296840	6.24%	1.622%
5	8.363	856	864	872	rBV	781962	1373251	28.87%	7.503%
6	9.203	997	1007	1019	rBV	625305	1163005	24.45%	6.354%
7	10.842	1278	1286	1302	rBV	190566	368558	7.75%	2.014%
8	13.286	1694	1702	1713	rBV	1818021	2828722	59.48%	15.455%
9	14.108	1837	1842	1856	rVB	130690	218438	4.59%	1.193%
10	14.660	1929	1936	1946	rBV2	354472	585003	12.30%	3.196%
11	15.947	2151	2155	2162	rVB	38479	47567	1.00%	0.260%
12	16.146	2183	2189	2202	rBV	964534	1545194	32.49%	8.442%
13	17.404	2393	2403	2421	rBV	526304	816736	17.17%	4.462%
14	20.012	2841	2847	2855	rBV	3427020	4756069	100.00%	25.985%
15	21.668	3122	3129	3142	rBV2	606959	1034191	21.74%	5.650%
16	23.149	3375	3381	3388	rBV3	37588	65574	1.38%	0.358%
17	23.948	3511	3517	3525	rVB3	43027	96648	2.03%	0.528%
18	24.876	3664	3675	3688	rBV2	359873	1048400	22.04%	5.728%
19	26.009	3861	3868	3878	rBV9	28558	83767	1.76%	0.458%


Sum of corrected areas: 18303178

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
Data File : BG035706.D
Acq On : 18 Jul 2018 7:04
Operator : JU/SJ
Sample : J3990-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

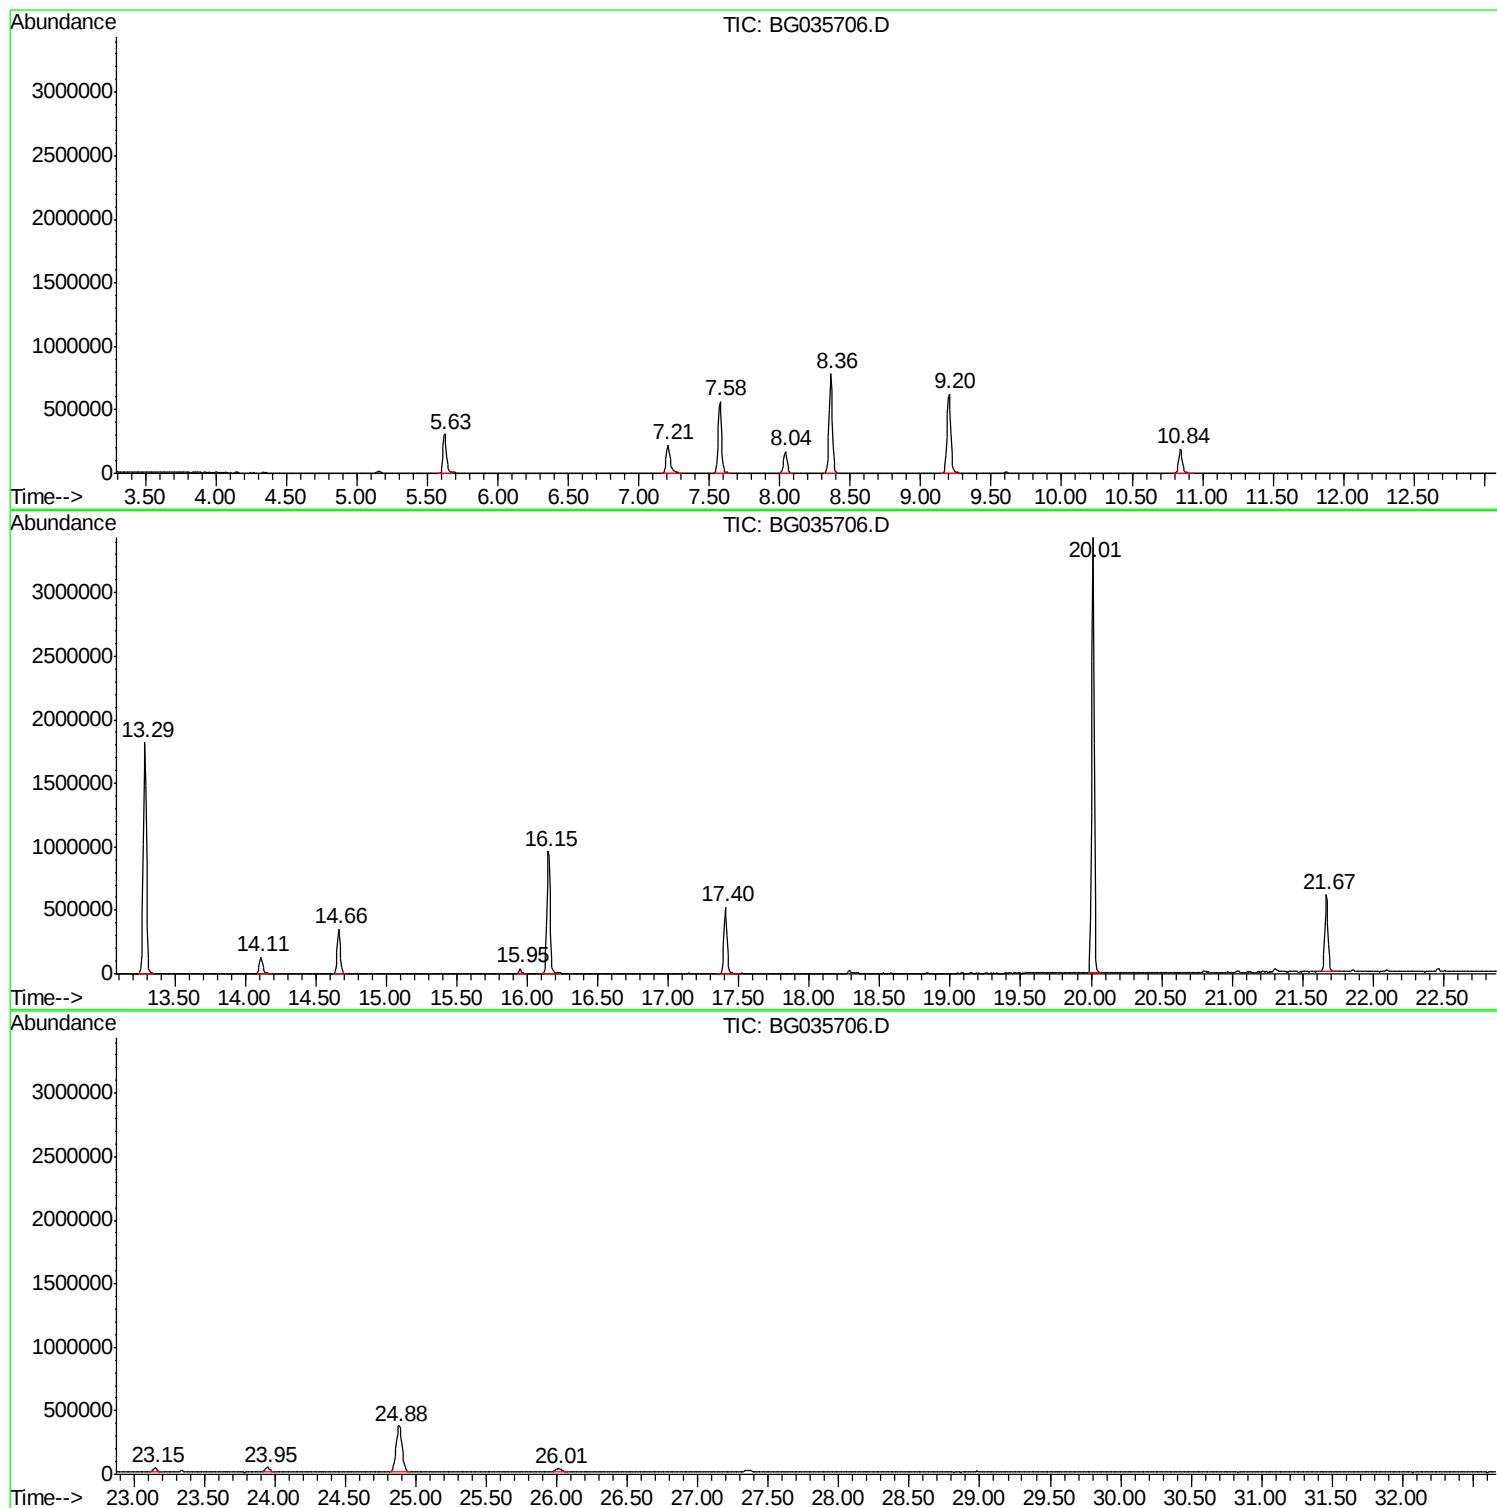

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data_File : BG035706.D
Acq_On : 18-Jul-2018 7:044
Operator : JU/SJJ
Sample : J3990-066
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
071218-DBRI-F-U-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
