

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
 Data File : BG035710.D
 Acq On : 18 Jul 2018 9:43
 Operator : JU/SJ
 Sample : J3990-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 071218-TIPC-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.622	390	397	410	rBV	351260	626755	12.95%	2.901%
2	7.209	659	667	681	rBV	263239	486976	10.06%	2.254%
3	7.573	721	729	741	rBV	603851	1076764	22.24%	4.984%
4	8.043	801	809	816	rBV	185238	327407	6.76%	1.516%
5	8.360	854	863	871	rBV	840968	1462116	30.20%	6.768%
6	9.200	998	1006	1019	rBV	665085	1222606	25.25%	5.660%
7	10.845	1278	1286	1296	rBV	204554	405813	8.38%	1.879%
8	13.289	1694	1702	1714	rBV	1757578	2897296	59.84%	13.412%
9	14.111	1836	1842	1849	rBV	86421	144643	2.99%	0.670%
10	14.663	1929	1936	1945	rBV2	371420	619539	12.80%	2.868%
11	15.950	2150	2155	2160	rBV	36278	49746	1.03%	0.230%
12	16.149	2182	2189	2199	rBV	1000888	1512924	31.25%	7.004%
13	17.406	2396	2403	2410	rBV2	525903	836853	17.29%	3.874%
14	18.288	2548	2553	2564	rBV2	85518	138085	2.85%	0.639%
15	19.557	2765	2769	2779	rBV3	35349	54946	1.13%	0.254%
16	20.015	2840	2847	2860	rBV	3562361	4841380	100.00%	22.411%
17	21.671	3122	3129	3143	rVB	651061	1095782	22.63%	5.073%
18	21.853	3155	3160	3166	rBV2	55167	73972	1.53%	0.342%
19	22.458	3256	3263	3268	rBV2	108296	177996	3.68%	0.824%
20	23.146	3373	3380	3387	rBV	199269	358969	7.41%	1.662%
21	23.945	3508	3516	3525	rBV	247034	517850	10.70%	2.397%
22	24.885	3665	3676	3690	rBV5	557165	1588326	32.81%	7.353%
23	26.012	3854	3868	3879	rBV2	186797	561981	11.61%	2.601%
24	27.352	4083	4096	4109	rBV5	105492	377255	7.79%	1.746%
25	28.973	4363	4372	4388	rVB7	33579	146322	3.02%	0.677%


Sum of corrected areas: 21602302

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071718\
Data File : BG035710.D
Acq On : 18 Jul 2018 9:43
Operator : JU/SJ
Sample : J3990-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
071218-TIPC-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

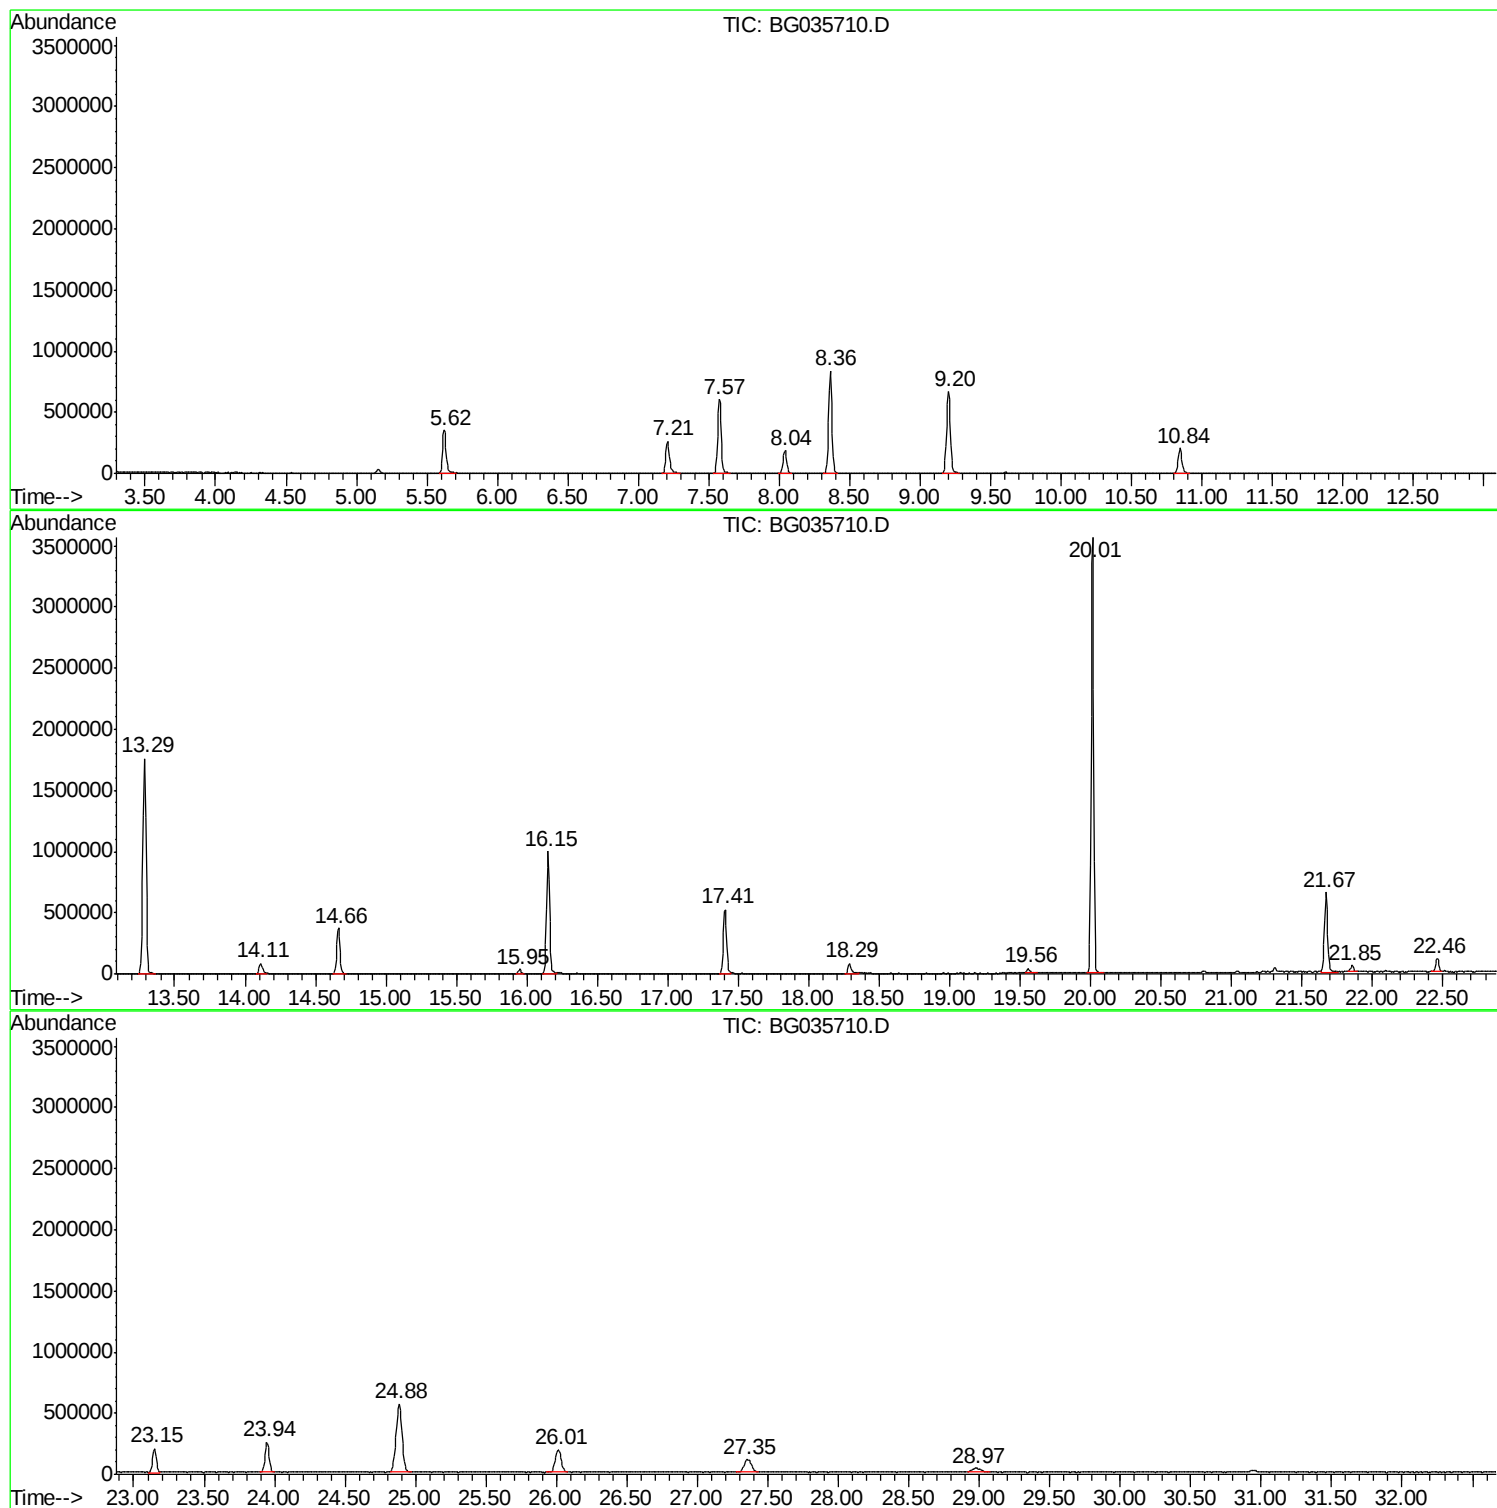

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071718\
Data_File : BG035710.D
Acq_On : 18-Jul-2018 9:433
Operator : JU/SJJ
Sample : J3990-100
Misc :
ALS_Vial : 29 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
071218-TIPC-F-U-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
