


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071718\
Data File : BG035680.D
Acq On : 17 Jul 2018 12:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 31 12:30:06 2018

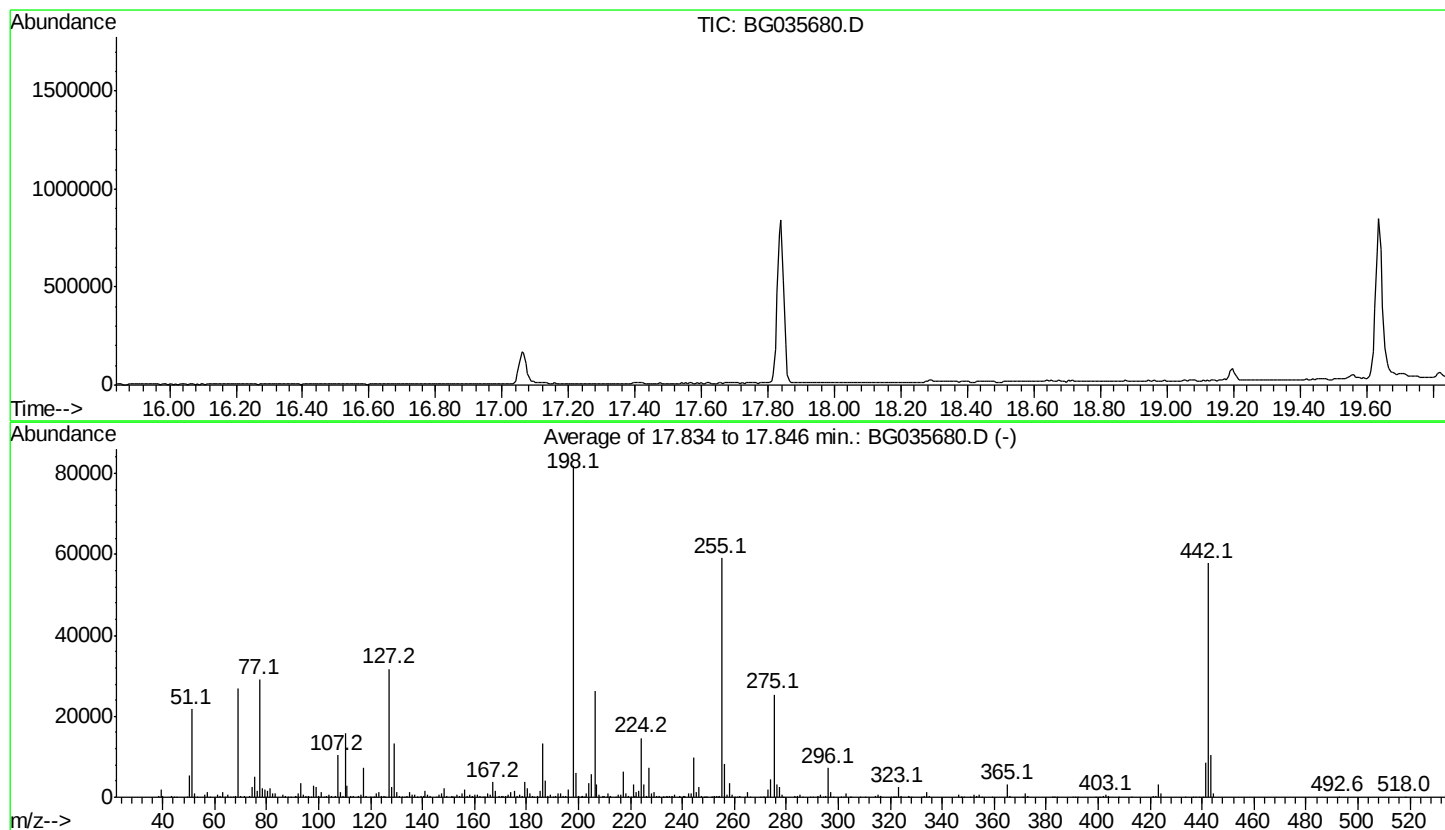

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	21709	PASS
68	69	0.00	2	0.7	200	PASS
69	198	0.00	100	32.8	26845	PASS
70	69	0.00	2	1.2	315	PASS
127	198	10	80	38.6	31642	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81949	PASS
199	198	5	9	7.4	6062	PASS
275	198	10	60	31.0	25400	PASS
365	198	1	100	3.7	3021	PASS
441	198	0.01	100	10.3	8481	PASS
442	198	50	100	70.5	57749	PASS
443	442	15	24	18.1	10439	PASS