


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071718\
 Data File : BG035699.D
 Acq On : 18 Jul 2018 2:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

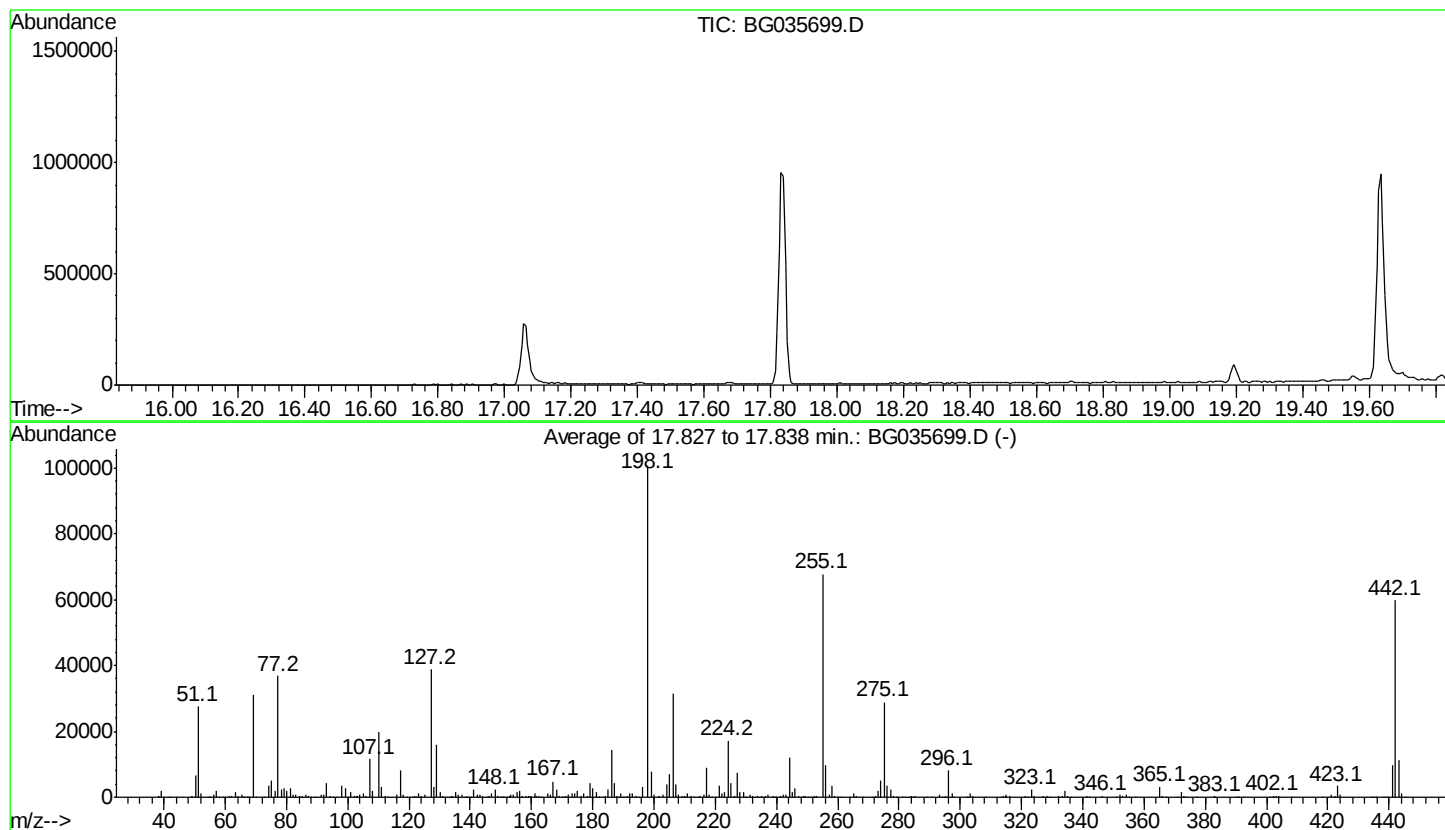

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	27482	PASS
68	69	0.00	2	0.5	153	PASS
69	198	0.00	100	31.0	31185	PASS
70	69	0.00	2	0.3	88	PASS
127	198	10	80	38.6	38861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100746	PASS
199	198	5	9	7.6	7621	PASS
275	198	10	60	28.7	28888	PASS
365	198	1	100	3.2	3194	PASS
441	198	0.01	100	9.5	9570	PASS
442	198	50	100	59.3	59730	PASS
443	442	15	24	19.0	11365	PASS