

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071719\
 Data File : BG041705.D
 Acq On : 18 Jul 2019 2:07
 Operator : HP/JU
 Sample : K3835-30
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-11(8-10)

Quant Time: Jul 18 07:12:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 15 16:16:21 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	97435	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	394557	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	241249	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	632418	20.00	ng	0.00
76) Chrysene-d12	21.65	240	658960	20.00	ng	-0.01
87) Perylene-d12	24.84	264	758119	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	659509	110.65	ng	0.00
7) Phenol-d6	7.20	99	918400	114.56	ng	0.00
23) Nitrobenzene-d5	9.20	82	540171	83.26	ng	-0.01
42) 2,4,6-Tribromophenol	16.14	330	351776	129.38	ng	0.00
45) 2-Fluorobiphenyl	13.29	172	1199438	76.99	ng	0.00
79) Terphenyl-d14	20.00	244	1940597	68.82	ng	0.00
Target Compounds						
9) Benzaldehyde	7.20	77	1715	Below Cal	Qvalue #	3
19) n-Nitroso-di-n-propylamine	9.20	70	72645	12.398 ng	#	74
50) Dimethylphthalate	14.11	163	254813	13.448 ng	#	97
57) 2,4-Dinitrotoluene	14.66	165	32127	6.047 ng	#	29
65) 4,6-Dinitro-2-methylphenol	16.14	198	1123	6.996 ng	#	1
67) 4-Bromophenyl-phenylether	16.14	248	27666	3.677 ng	#	1
77) Benizidine	20.00	184	33426	Below Cal	#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071719\
Data File : BG041705.D
Acq On : 18 Jul 2019 2:07
Operator : HP/JU
Sample : K3835-30
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-11(8-10)

Quant Time: Jul 18 07:12:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

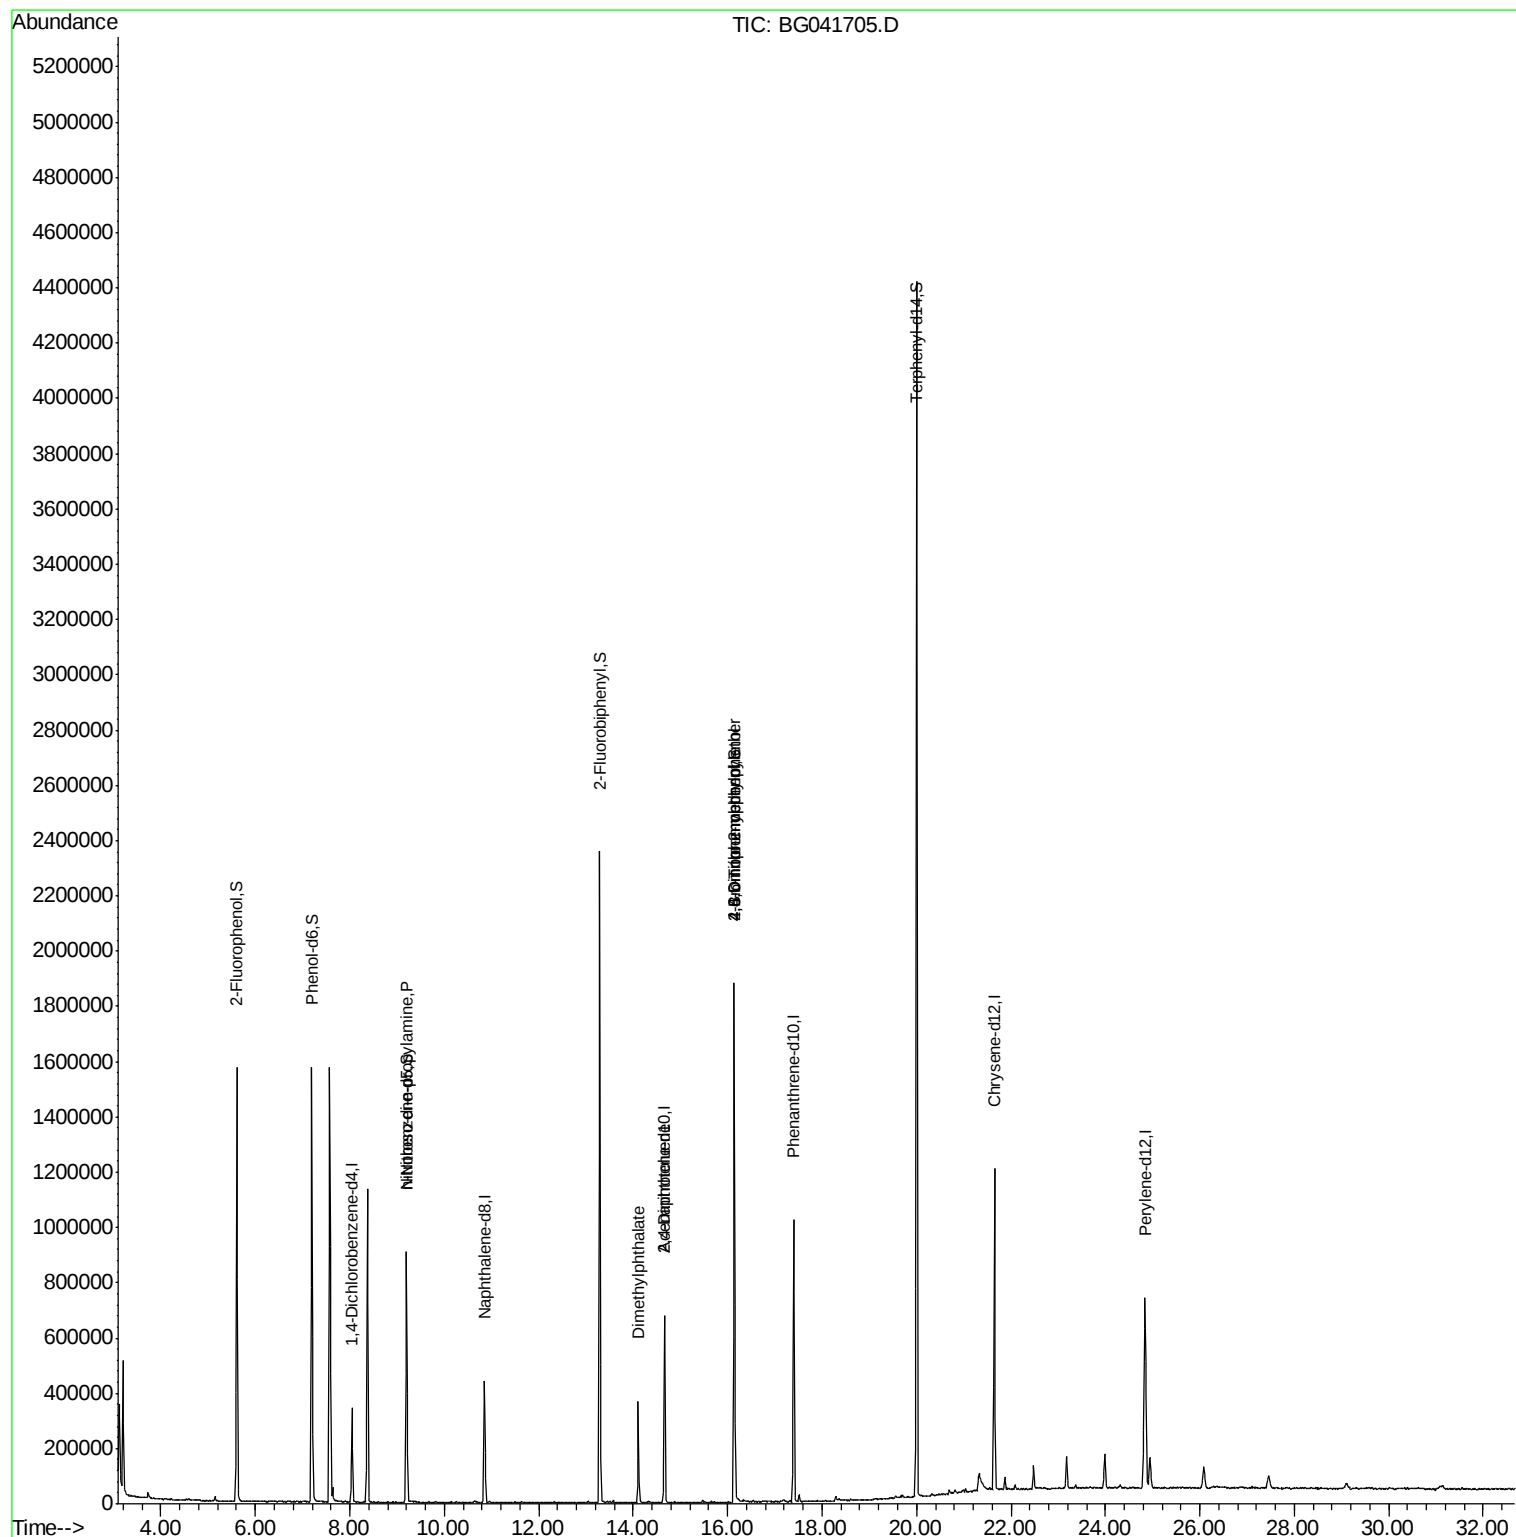

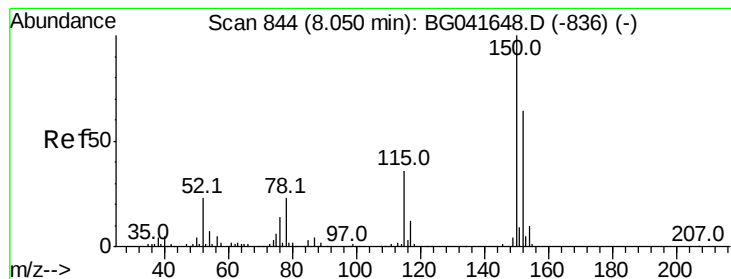


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.01 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07

Instrument :
BNA_G
ClientSampleId :
SB-11(8-10)

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.9	126.9	190.3
115	53.7	45.0	67.6



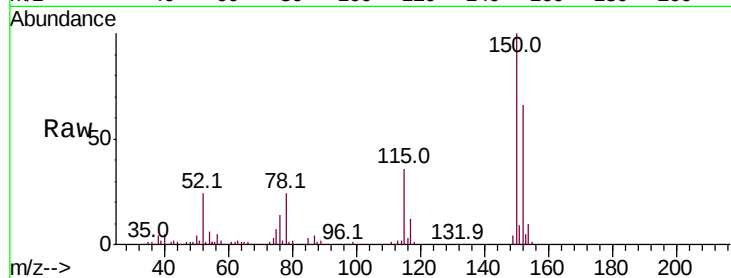


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

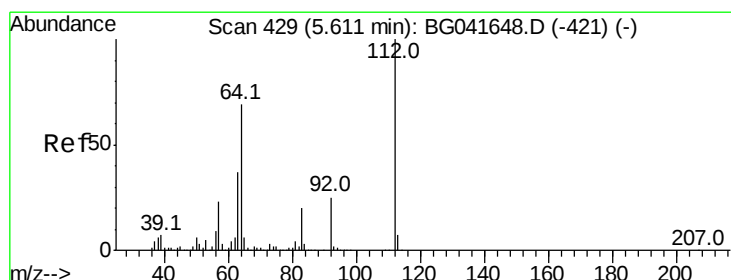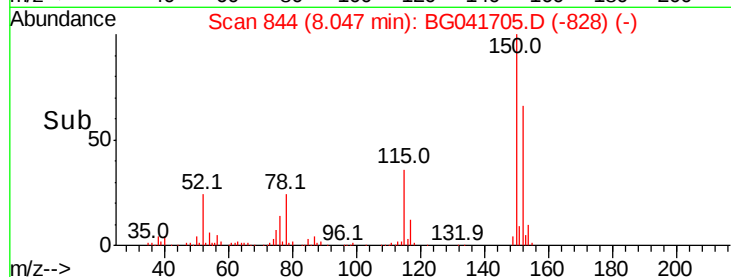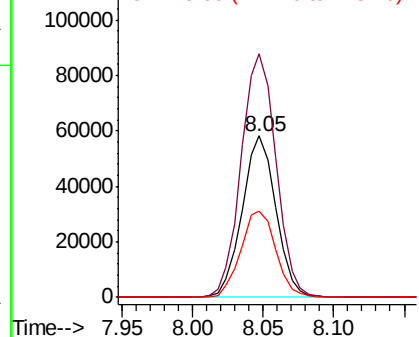

#5

2-Fluorophenol
Concen: 110.651 ng
RT: 5.61 min Scan# 429
Delta R.T. -0.00 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.6	55.4	83.2
63	36.3	29.1	43.7


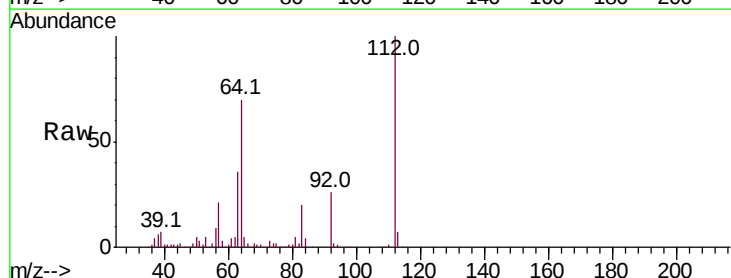



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

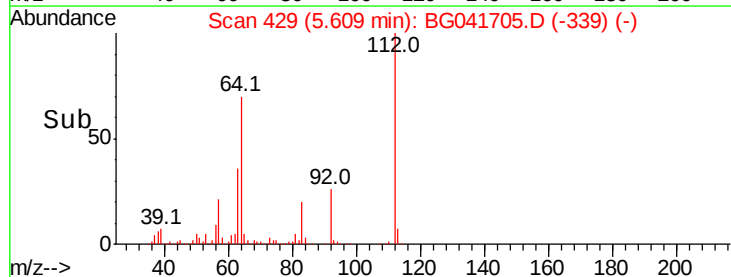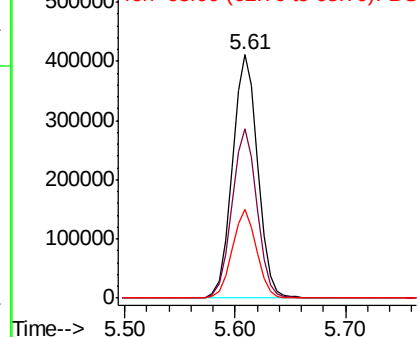

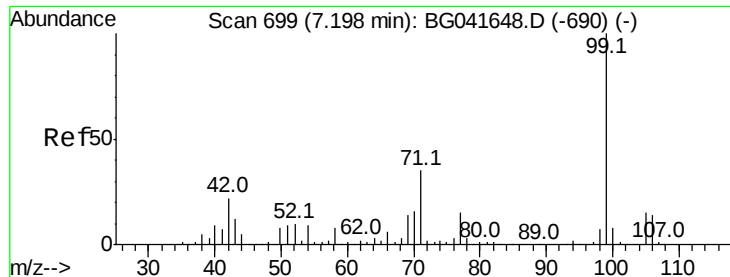

#7

Phenol-d6

Concen: 114.560 ng

RT: 7.20 min Scan# 699

Delta R.T. -0.01 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07

Instrument :

BNA_G

ClientSampleId :

SB-11(8-10)


Tot Ion: 99 Resp: 918400

Ion Ratio Lower Upper




99 100

42 21.0 17.6 26.4

71 34.9 27.8 41.6

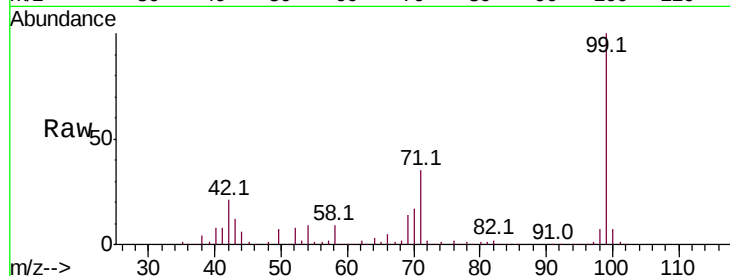

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

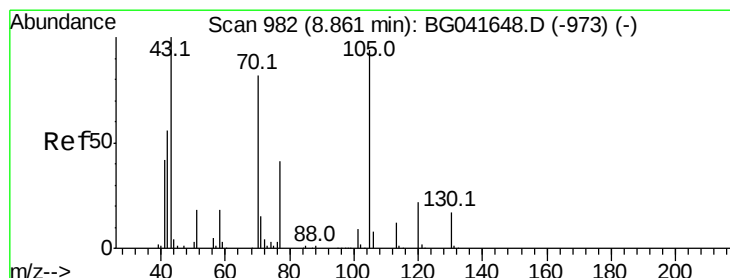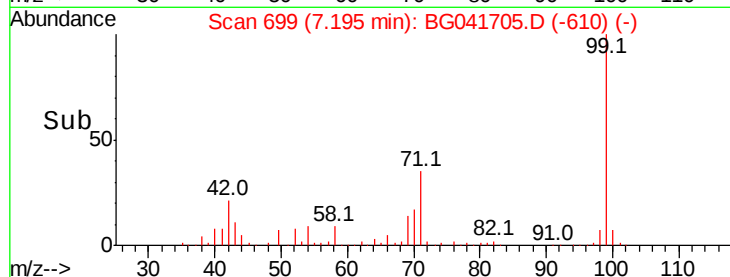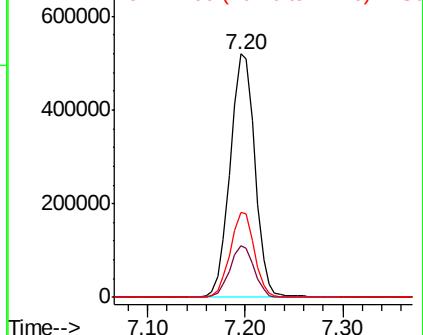

#19

n-Nitroso-di-n-propylamine

Concen: 12.398 ng

RT: 9.20 min Scan# 1040

Delta R.T. 0.33 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07

Tgt Ion: 70 Resp: 72645


Ion Ratio Lower Upper

70 100



42 52.7 55.8 83.6#


101 0.0 8.1 12.1#

130 1.9 17.3 25.9#

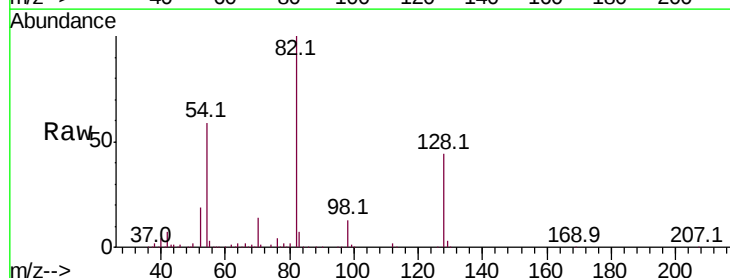

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

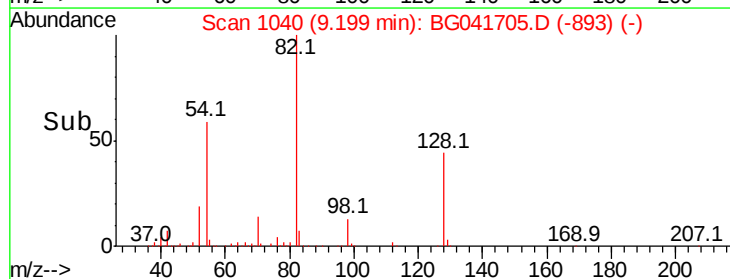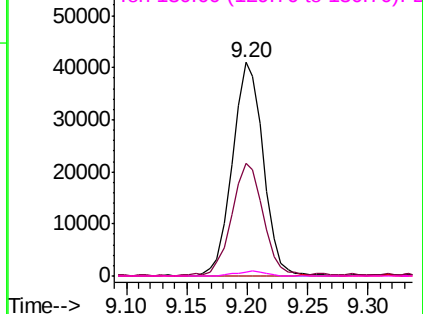

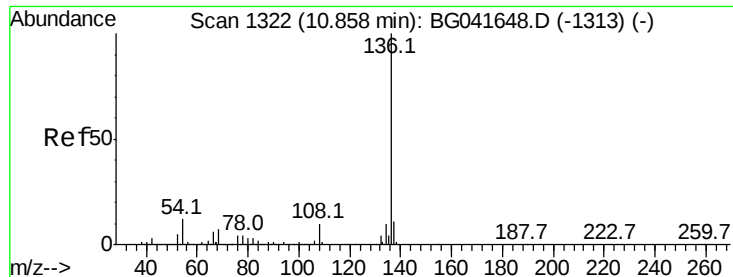

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1321

Delta R.T. -0.01 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07

Instrument :

BNA_G

ClientSampleId :

SB-11(8-10)

Tot Ion:136 Resp: 394557



Ion Ratio Lower Upper

136 100



137 11.4 9.2 13.8

54 10.0 8.7 13.1

68 5.9 5.5 8.3

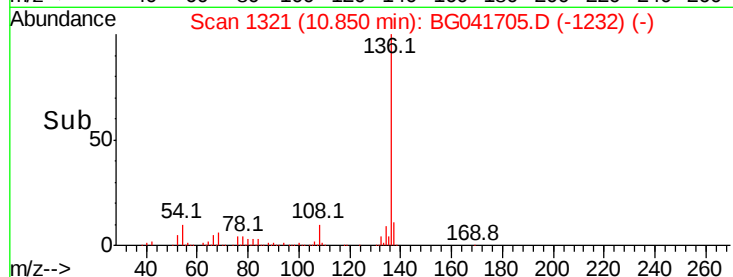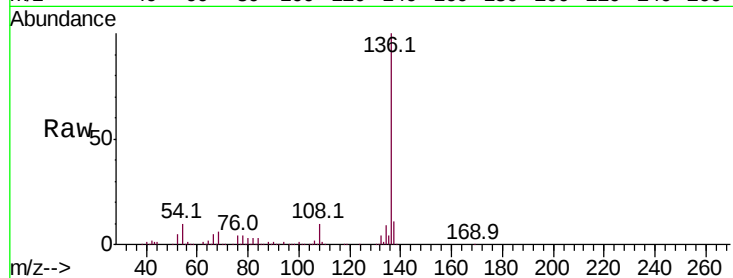

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

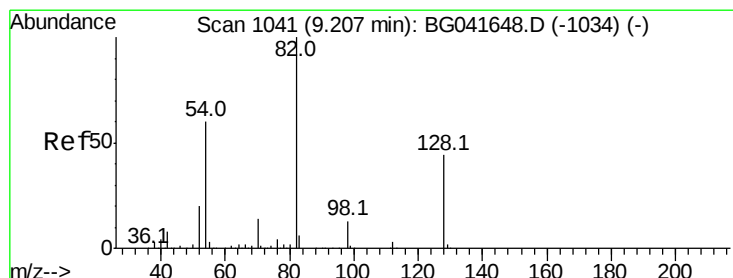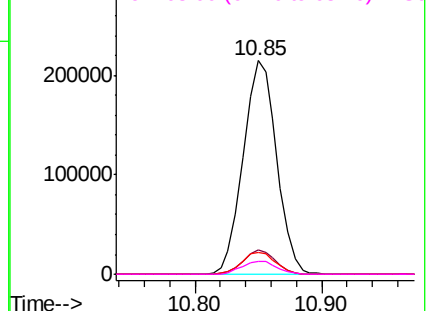

#23

Nitrobenzene-d5

Concen: 83.259 ng

RT: 9.20 min Scan# 1040

Delta R.T. -0.01 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07



Tgt Ion: 82 Resp: 540171

Ion Ratio Lower Upper


82 100


128 44.3 35.1 52.7

54 58.9 48.7 73.1

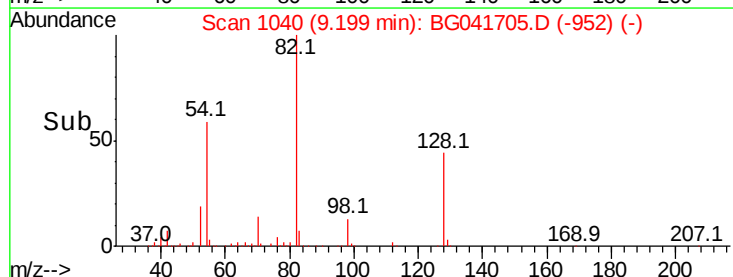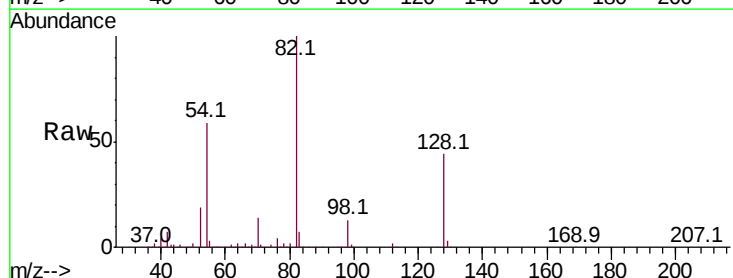

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC




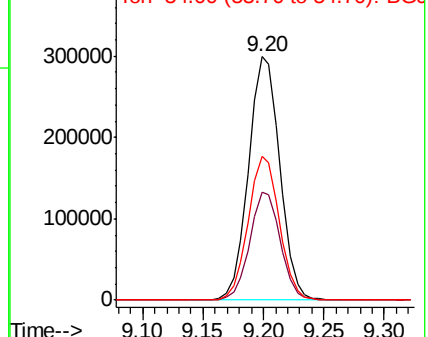


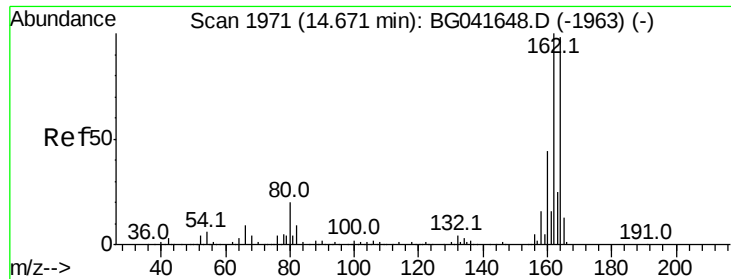

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.66 min Scan# 1970
Delta R.T. -0.01 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07




Instrument :
BNA_G
ClientSampleId :
SB-11(8-10)


Tot Ion	Ratio	Lower	Upper
164	100		
162	104.2	79.6	119.4
160	44.2	35.4	53.0

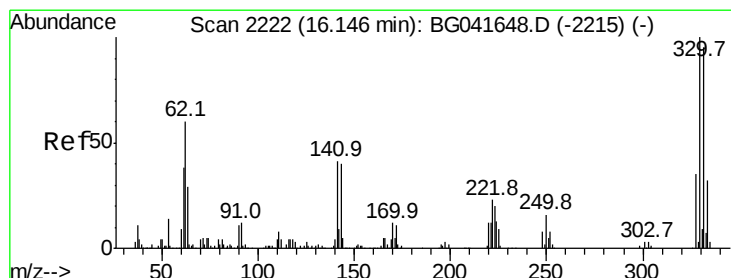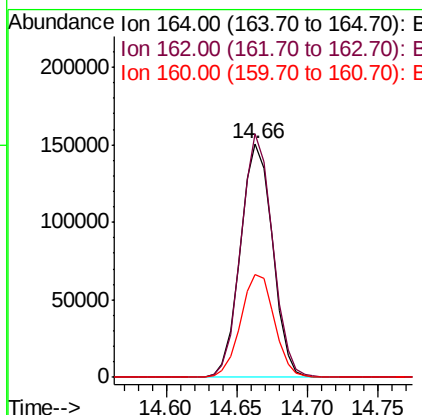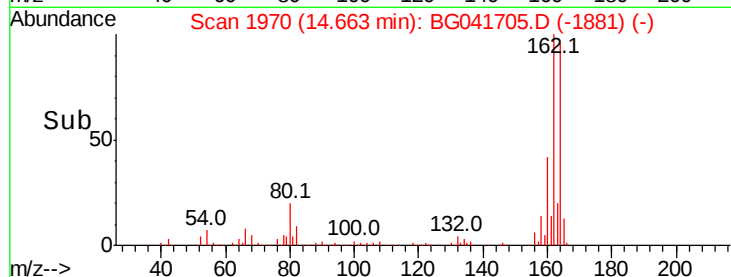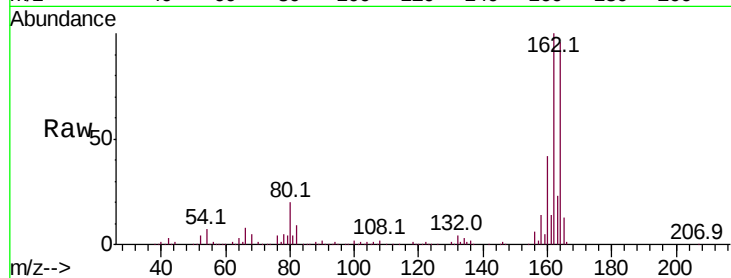

#42
2,4,6-Tribromophenol
Concen: 129.385 ng
RT: 16.14 min Scan# 2222
Delta R.T. -0.01 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.4	116.0
141	39.4	31.9	47.9

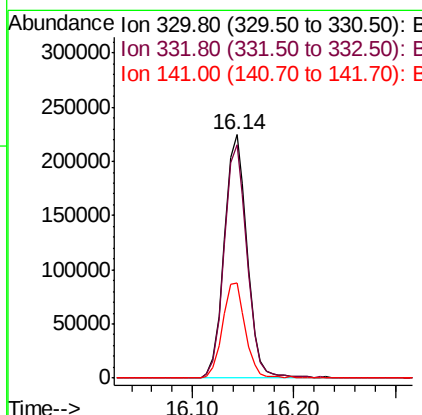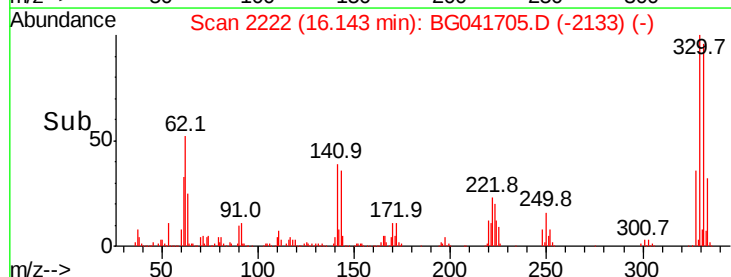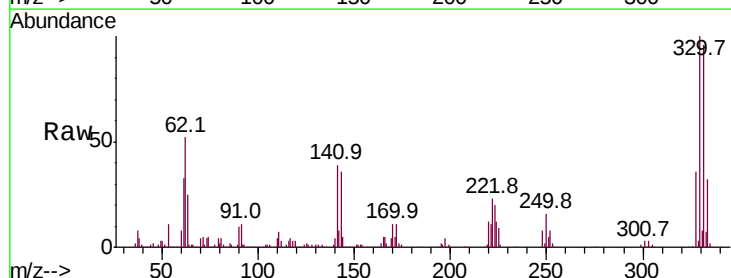


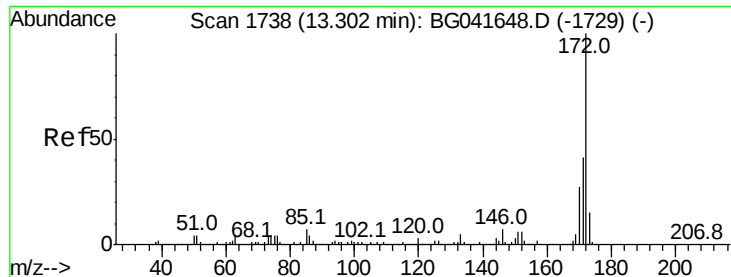




#45
2-Fluorobiphenyl
Concen: 76.988 ng
RT: 13.29 min Scan# 1737
Delta R.T. -0.01 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07

Instrument :
BNA_G
ClientSampleId :
SB-11(8-10)

Tot Ion:172 Resp: 1199438
Ion Ratio Lower Upper
172 100
171 39.7 35.0 52.4
170 26.3 23.5 35.3

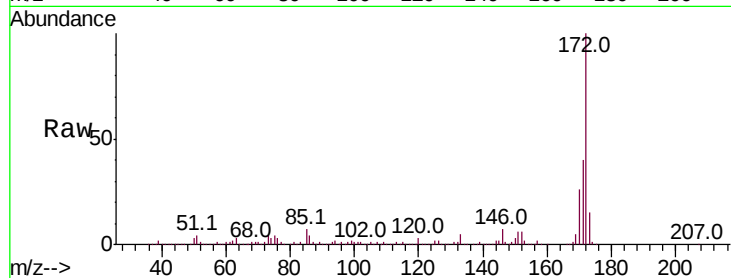


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

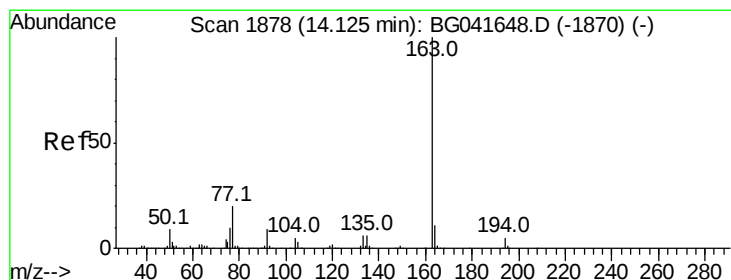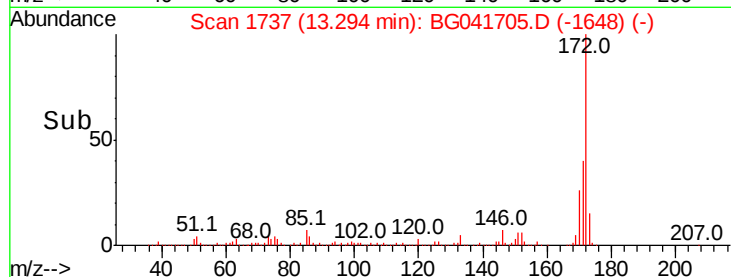
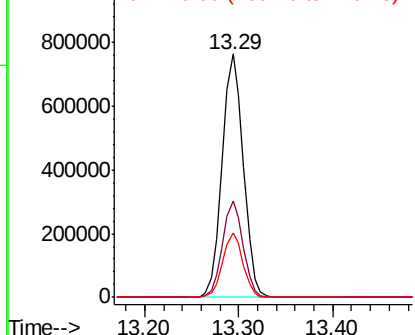



#50
Dimethylphthalate
Concen: 13.448 ng
RT: 14.11 min Scan# 1876
Delta R.T. -0.02 min
Lab File: BG041705.D
Acq: 18 Jul 2019 2:07

Tgt Ion:163 Resp: 254813
Ion Ratio Lower Upper
163 100
194 4.6 4.2 6.2
164 10.2 9.4 14.2

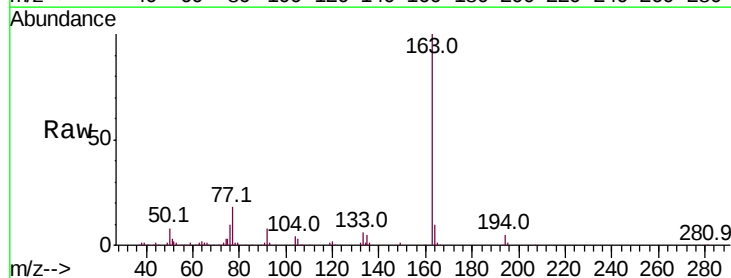

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

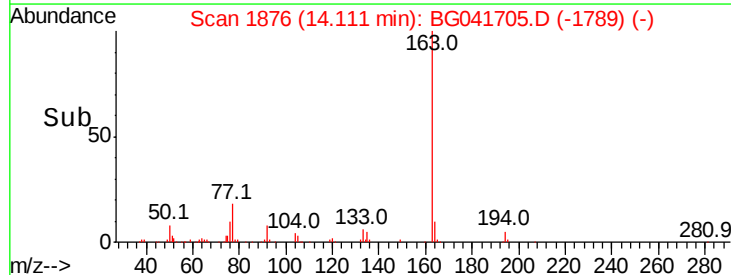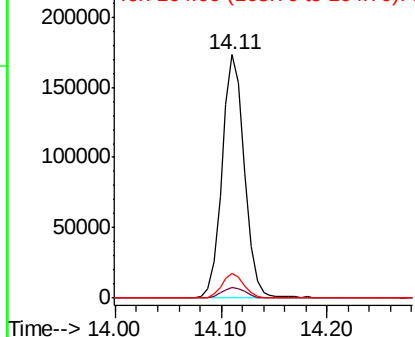


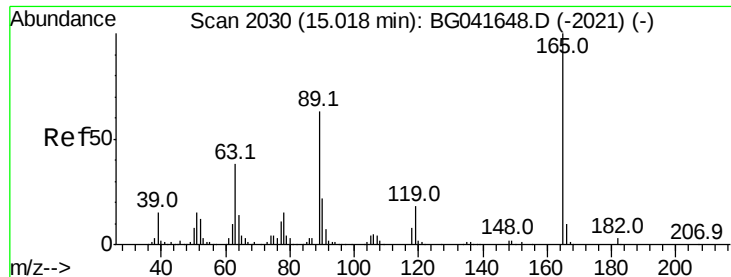




#57
 2,4-Dinitrotoluene
 Concen: 6.047 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. -0.36 min
 Lab File: BG041705.D
 Acq: 18 Jul 2019 2:07

Instrument :
 BNA_G
 ClientSampleId :
 SB-11(8-10)

Tot Ion:165 Resp: 32127
 Ion Ratio Lower Upper
 165 100
 63 1.3 31.7 47.5#
 89 0.8 50.2 75.4#
 182 0.0 2.6 4.0#

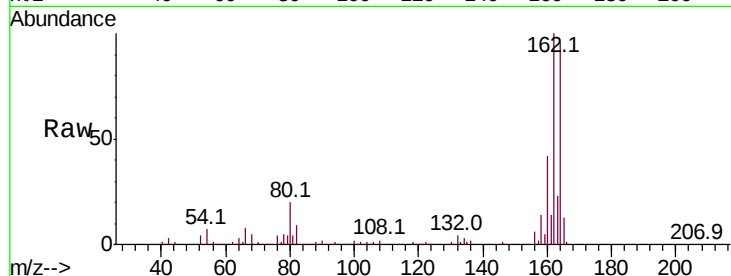


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

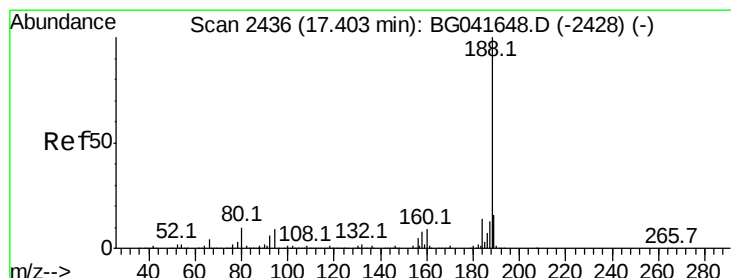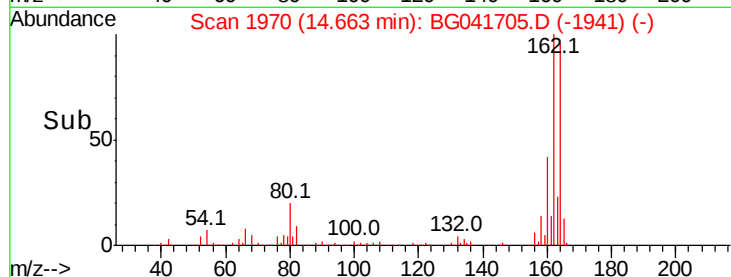
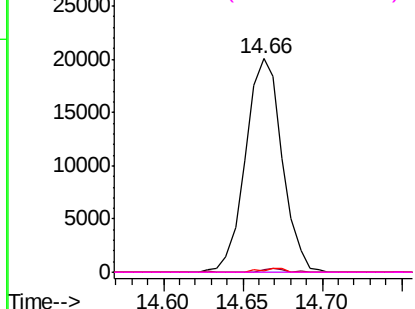



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.40 min Scan# 2436
 Delta R.T. -0.01 min
 Lab File: BG041705.D
 Acq: 18 Jul 2019 2:07

Tgt Ion:188 Resp: 632418
 Ion Ratio Lower Upper
 188 100
 94 8.2 6.9 10.3
 80 9.1 8.0 12.0

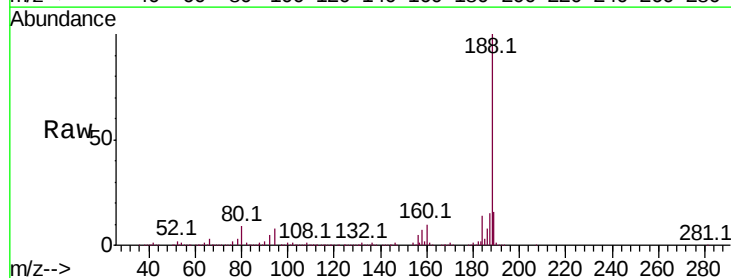

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

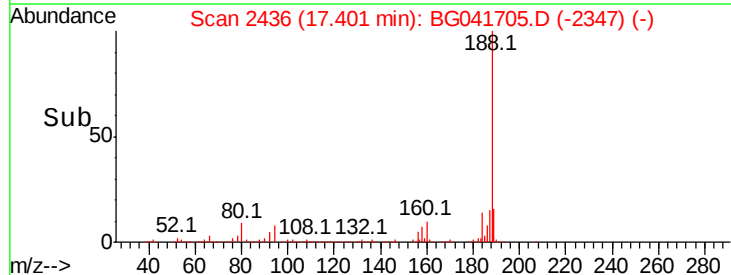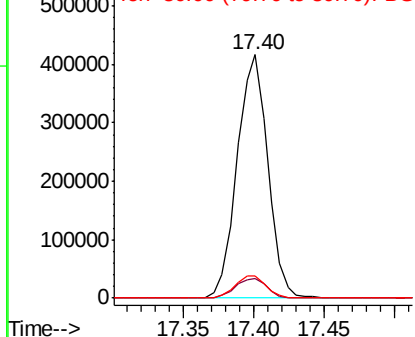


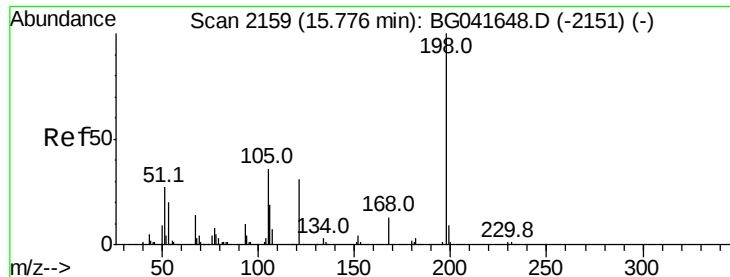




#65
 4,6-Dinitro-2-methylphenol
 Concen: 6.996 ng
 RT: 16.14 min Scan# 2222
 Delta R.T. 0.36 min
 Lab File: BG041705.D
 Acq: 18 Jul 2019 2:07

Instrument :
 BNA_G
 ClientSampleId :
 SB-11(8-10)

Tot Ion:198 Resp: 1123
 Ion Ratio Lower Upper
 198 100
 51 123.0 22.3 62.3#
 105 144.1 18.0 58.0#

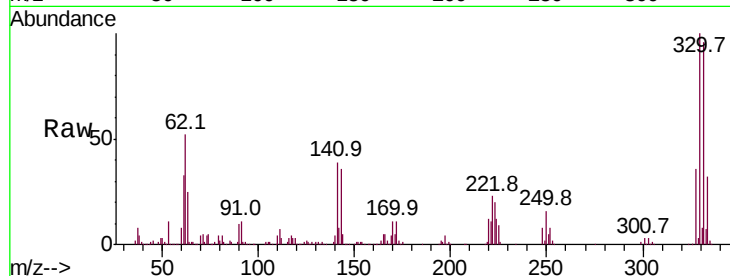


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG0
 Ion 105.00 (104.70 to 105.70): E

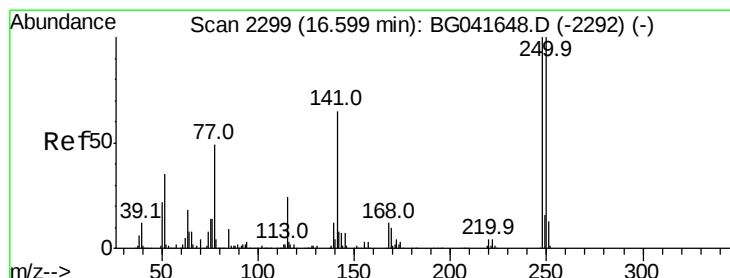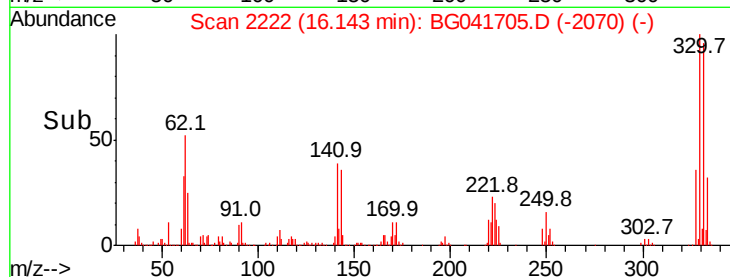
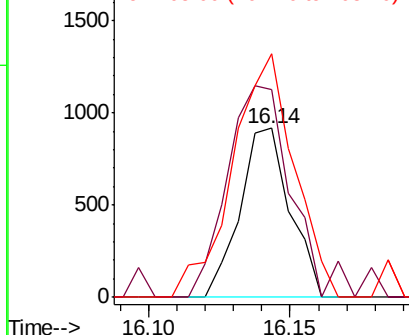



#67
 4-Bromophenyl-phenylether
 Concen: 3.677 ng
 RT: 16.14 min Scan# 2221
 Delta R.T. -0.47 min
 Lab File: BG041705.D
 Acq: 18 Jul 2019 2:07

Tgt Ion:248 Resp: 27666
 Ion Ratio Lower Upper
 248 100
 250 186.2 78.1 117.1#
 141 484.9 49.6 74.4#

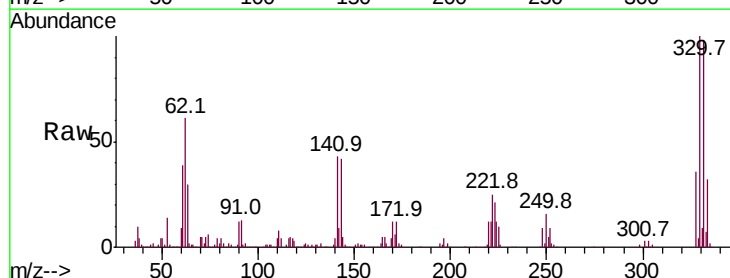

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

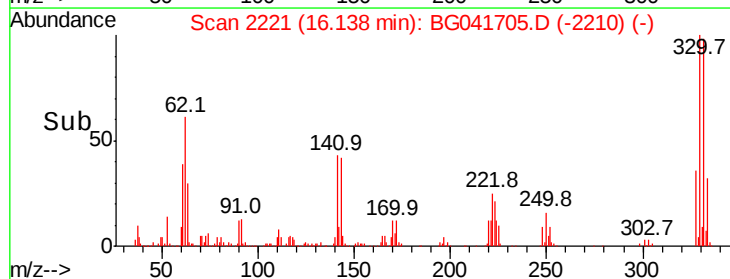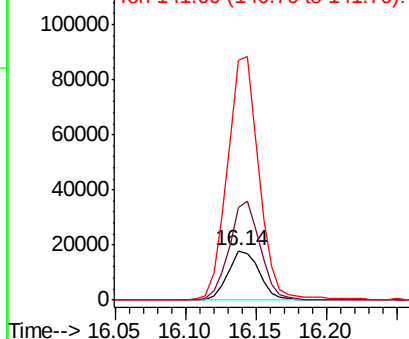

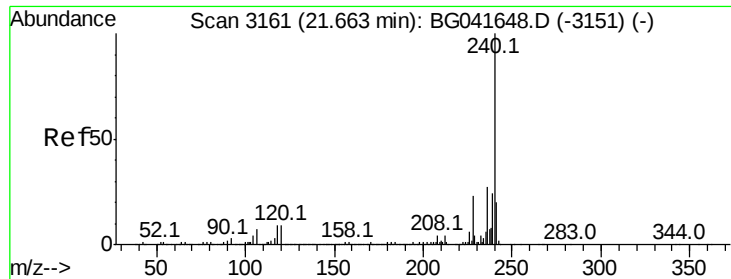

#76

Chrvsene-d12

Concen: 20.000 ng

RT: 21.65 min Scan# 3159

Delta R.T. -0.01 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07

Instrument :

BNA_G

ClientSampleId :

SB-11(8-10)


Tot Ion:240 Resp: 658960

Ion Ratio Lower Upper

240 100

120 9.7 8.0 12.0




236 28.0 22.6 33.8

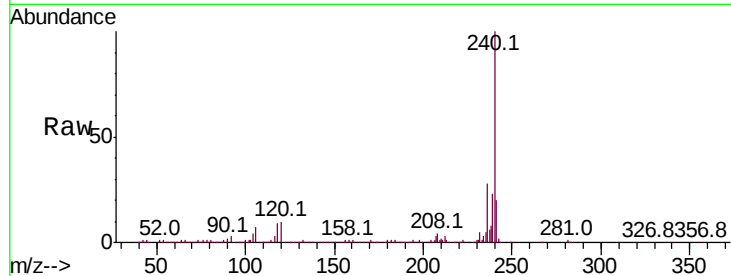

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

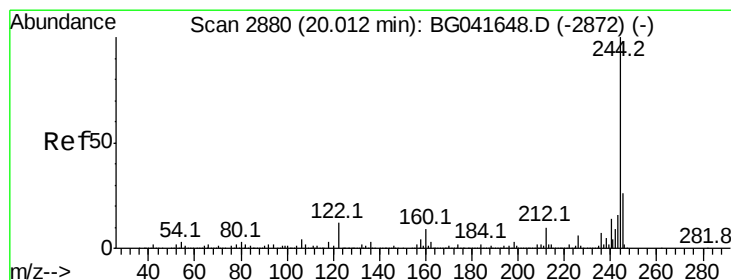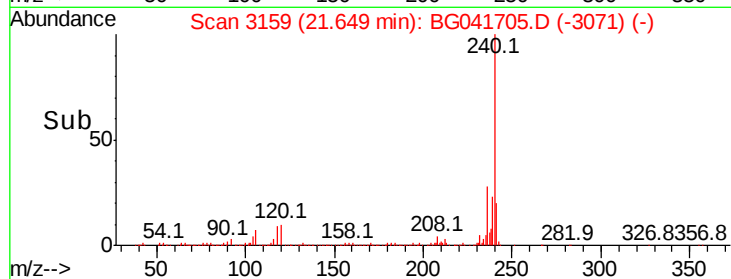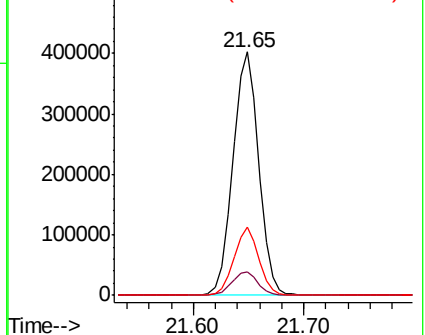

#79

Terphenyl-d14

Concen: 68.820 ng

RT: 20.00 min Scan# 2879

Delta R.T. -0.01 min

Lab File: BG041705.D

Acq: 18 Jul 2019 2:07


Tgt Ion:244 Resp: 1940597

Ion Ratio Lower Upper

244 100

212 9.7 9.7 14.5



122 12.4 12.5 18.7#

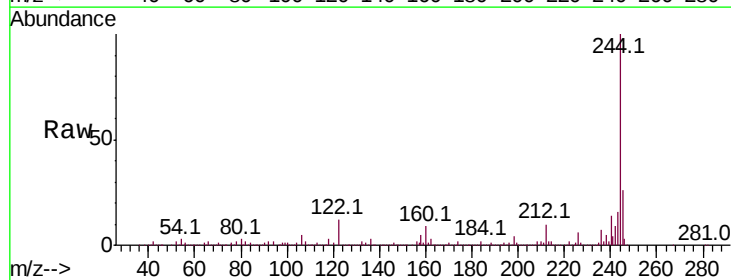


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

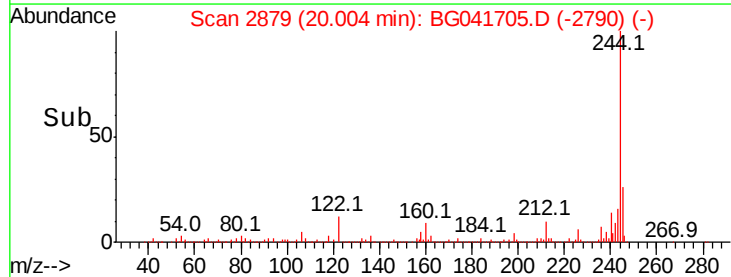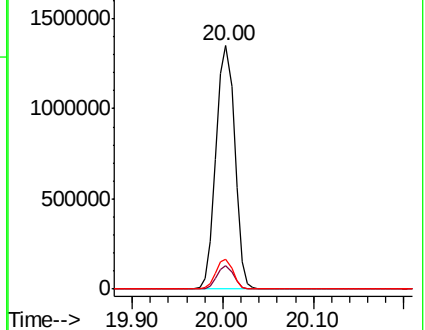


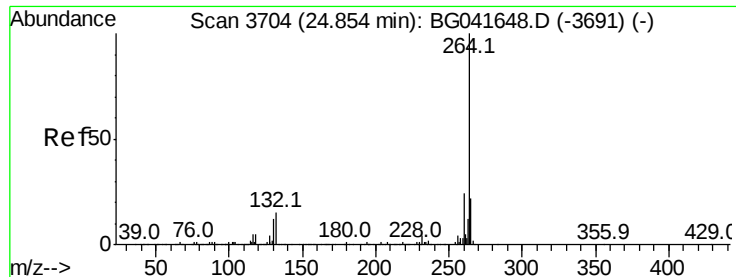

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.84 min Scan# 3702
 Delta R.T. -0.02 min
 Lab File: BG041705.D
 Acq: 18 Jul 2019 2:07

Instrument :
 BNA_G
 ClientSampleId :
 SB-11(8-10)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.5	29.3
265	22.5	18.0	27.0

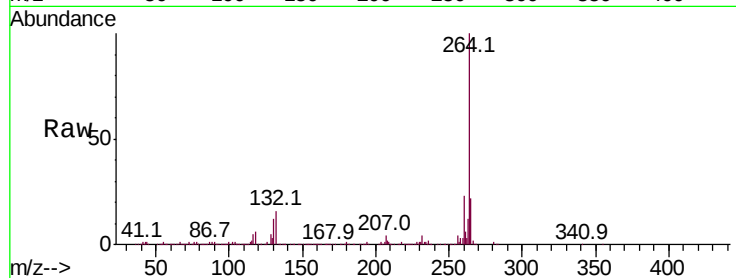

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

