
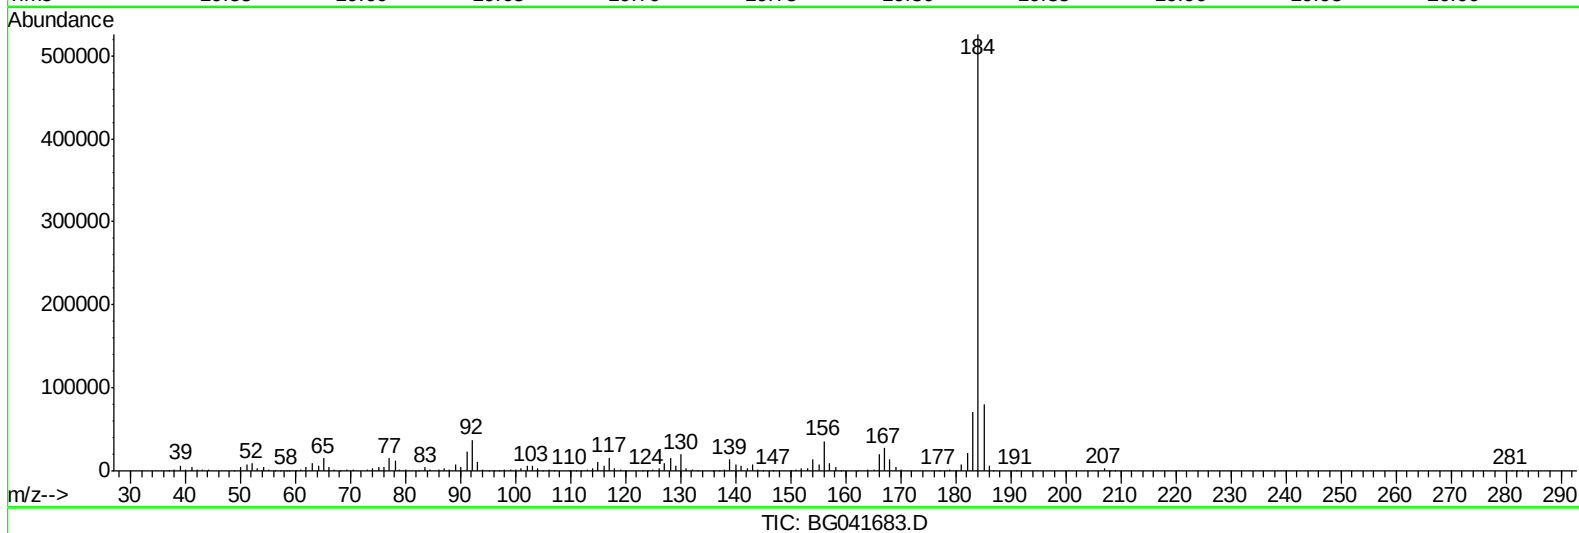


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071719\
Data File : BG041683.D
Acq On : 17 Jul 2019 10:48
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 08:58:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

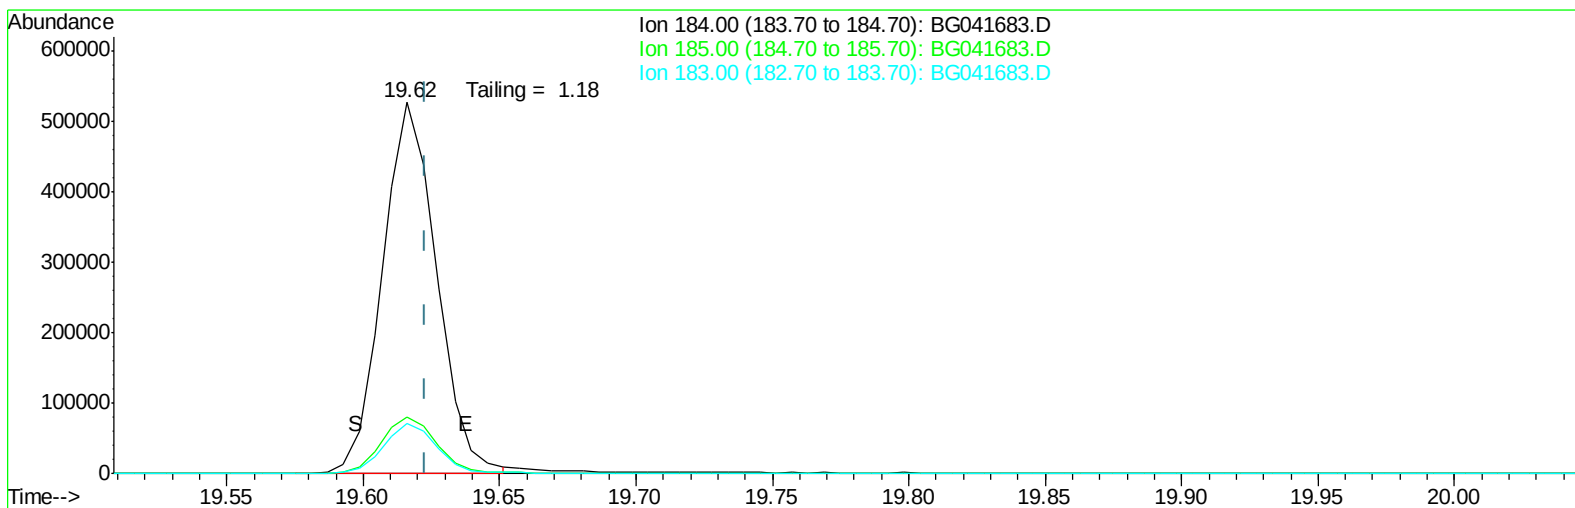

(77) Benzidine



19.616min (-0.007) 0.00ng

response 737315

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.33
183.00	14.70	13.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071719\
Data File : BG041683.D
Acq On : 17 Jul 2019 10:48
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 08:58:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

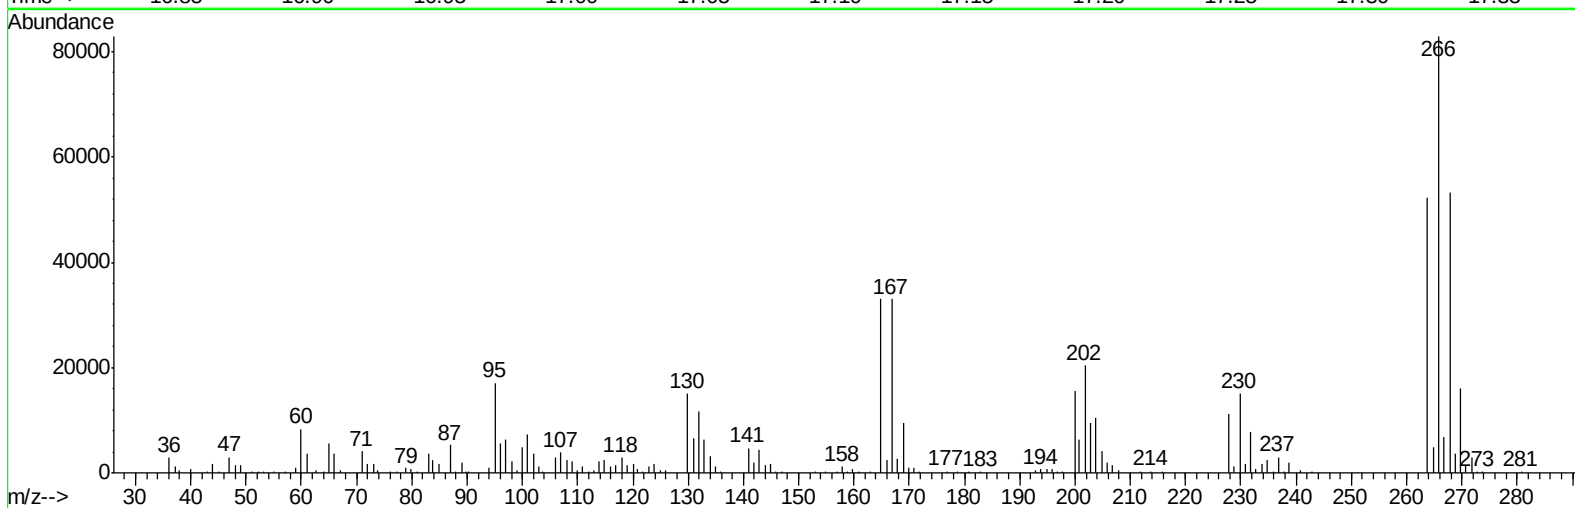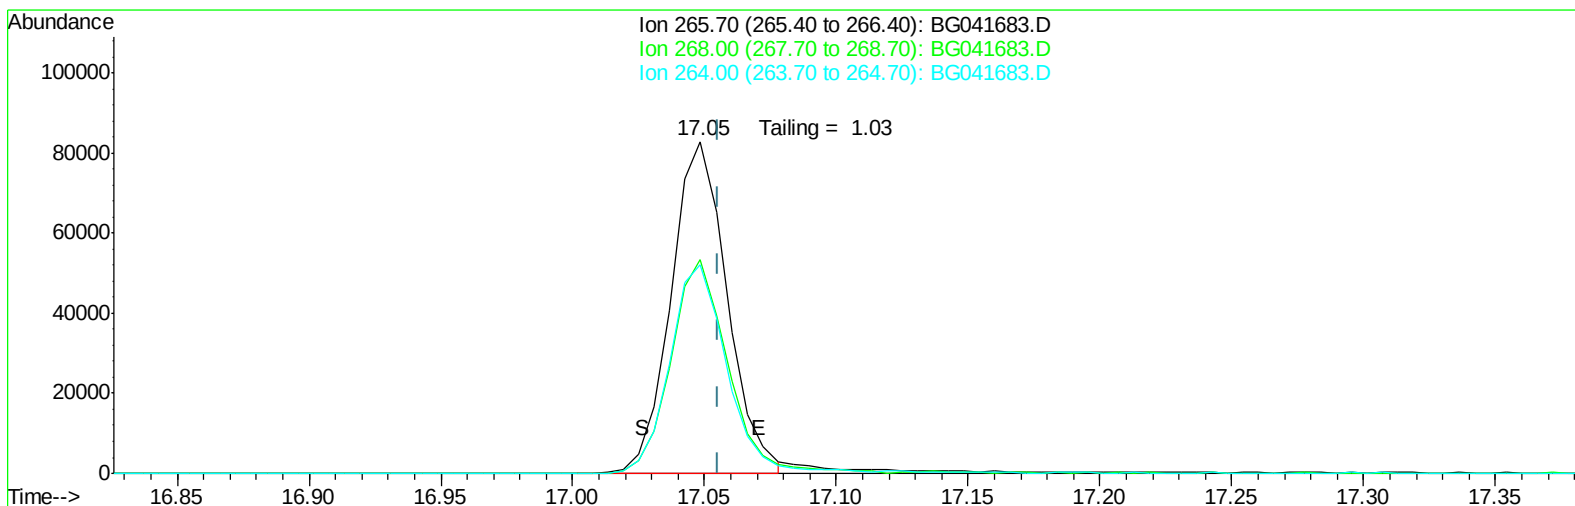

TIC: BG041683.D

(70) Pentachlorophenol (C)

17.049min (-0.007) 28346.96ng

response 125086

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	64.23
264.00	64.30	62.98
0.00	0.00	0.00