


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071719\
 Data File : BG041683.D
 Acq On : 17 Jul 2019 10:48
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

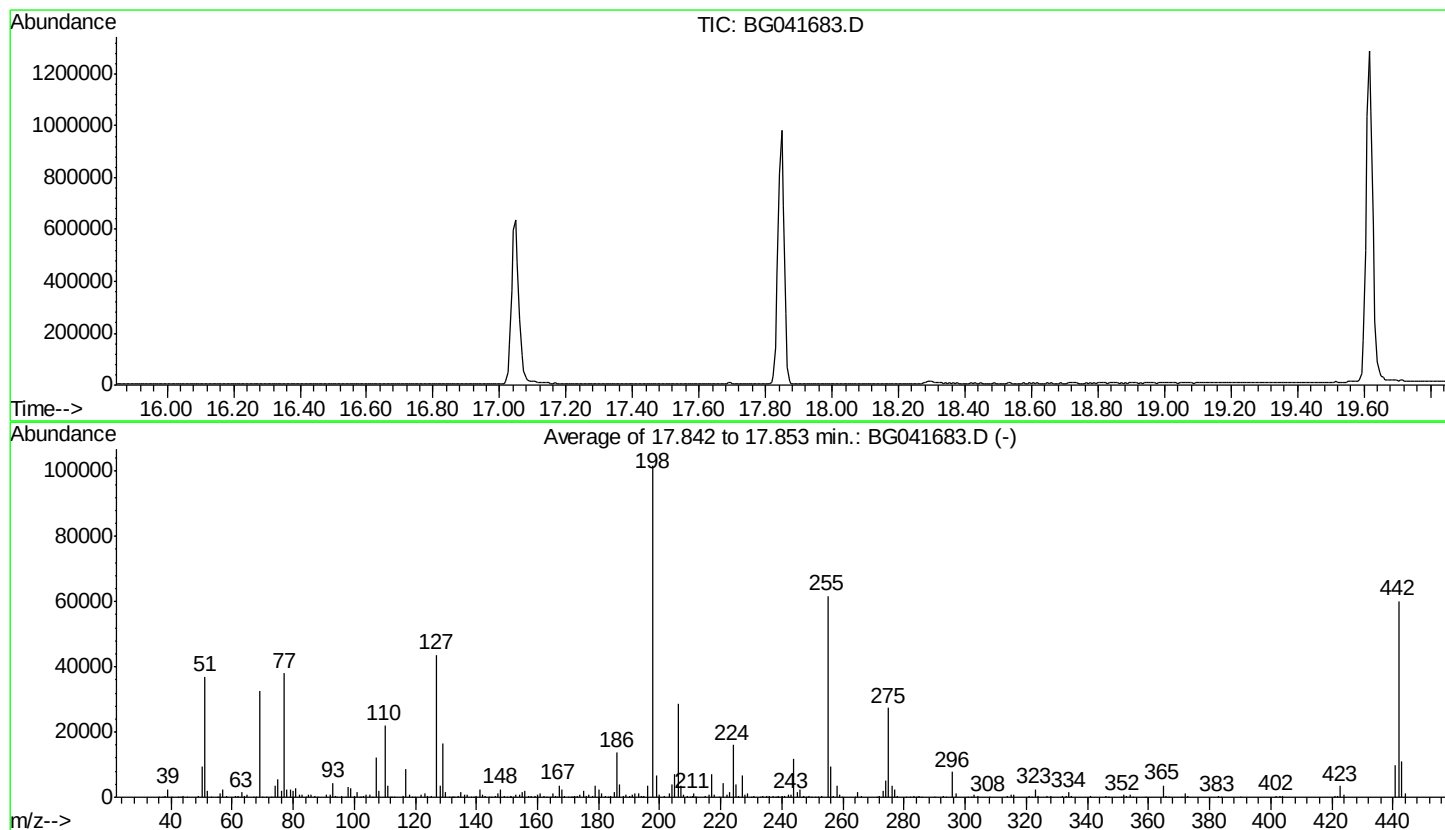

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	36970	PASS
68	69	0.00	2	0.6	186	PASS
69	198	0.00	100	31.9	32469	PASS
70	69	0.00	2	0.5	174	PASS
127	198	10	80	42.9	43584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101706	PASS
199	198	5	9	6.7	6790	PASS
275	198	10	60	27.0	27453	PASS
365	198	1	100	3.5	3607	PASS
441	198	0.01	100	9.6	9758	PASS
442	198	50	100	59.2	60189	PASS
443	442	15	24	18.6	11169	PASS