

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
 Data File : BG062119.D
 Acq On : 17 Jul 2024 19:11
 Operator : MA/JU
 Sample : P3217-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YDZG5

Quant Time: Jul 18 01:06:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 16 12:23:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	22156	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	101187	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.676	164	71040	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.420	188	171752	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.680	240	148867	20.000	ng/ul	#-0.01
88) Perylene-d12	24.906	264	177015	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.437	96	1962	3.328	ng/uL	0.00
4) Pyridine-d5	3.860	84	14529	8.014	ng/ul	0.00
7) Phenol-d5	7.220	99	18775	7.743	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.367	67	34064	22.185	ng/ul	0.00
11) 2-Chlorophenol-d4	7.579	132	42510	25.559	ng/ul	0.00
15) 4-Methylphenol-d8	8.760	113	32013	16.769	ng/ul	0.00
21) Nitrobenzene-d5	9.206	128	26207	34.054	ng/ul	-0.02
24) 2-Nitrophenol-d4	9.941	143	31046	35.327	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	58026	34.232	ng/ul	0.00
31) 4-Chloroaniline-d4	10.993	131	56393	22.915	ng/ul	-0.01
46) Dimethylphthalate-d6	14.077	166	197854	33.877	ng/ul	0.00
49) Acenaphthylene-d8	14.371	160	216987	35.531	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.911	143	7260	7.784	ng/ul	0.00
60) Fluorene-d10	15.669	176	181433	36.901	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	29753	32.985	ng/ul	-0.01
73) Anthracene-d10	17.520	188	272626	33.998	ng/ul	0.00
81) Pyrene-d10	19.806	212	309838	35.385	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.682	264	315041	35.886	ng/ul	-0.01
Target Compounds						
					Qvalue	
23) Isophorone	9.935	82	5498	1.114	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
Data File : BG062119.D
Acq On : 17 Jul 2024 19:11
Operator : MA/JU
Sample : P3217-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YDZG5

Quant Time: Jul 18 01:06:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 16 12:23:16 2024
Response via : Initial Calibration

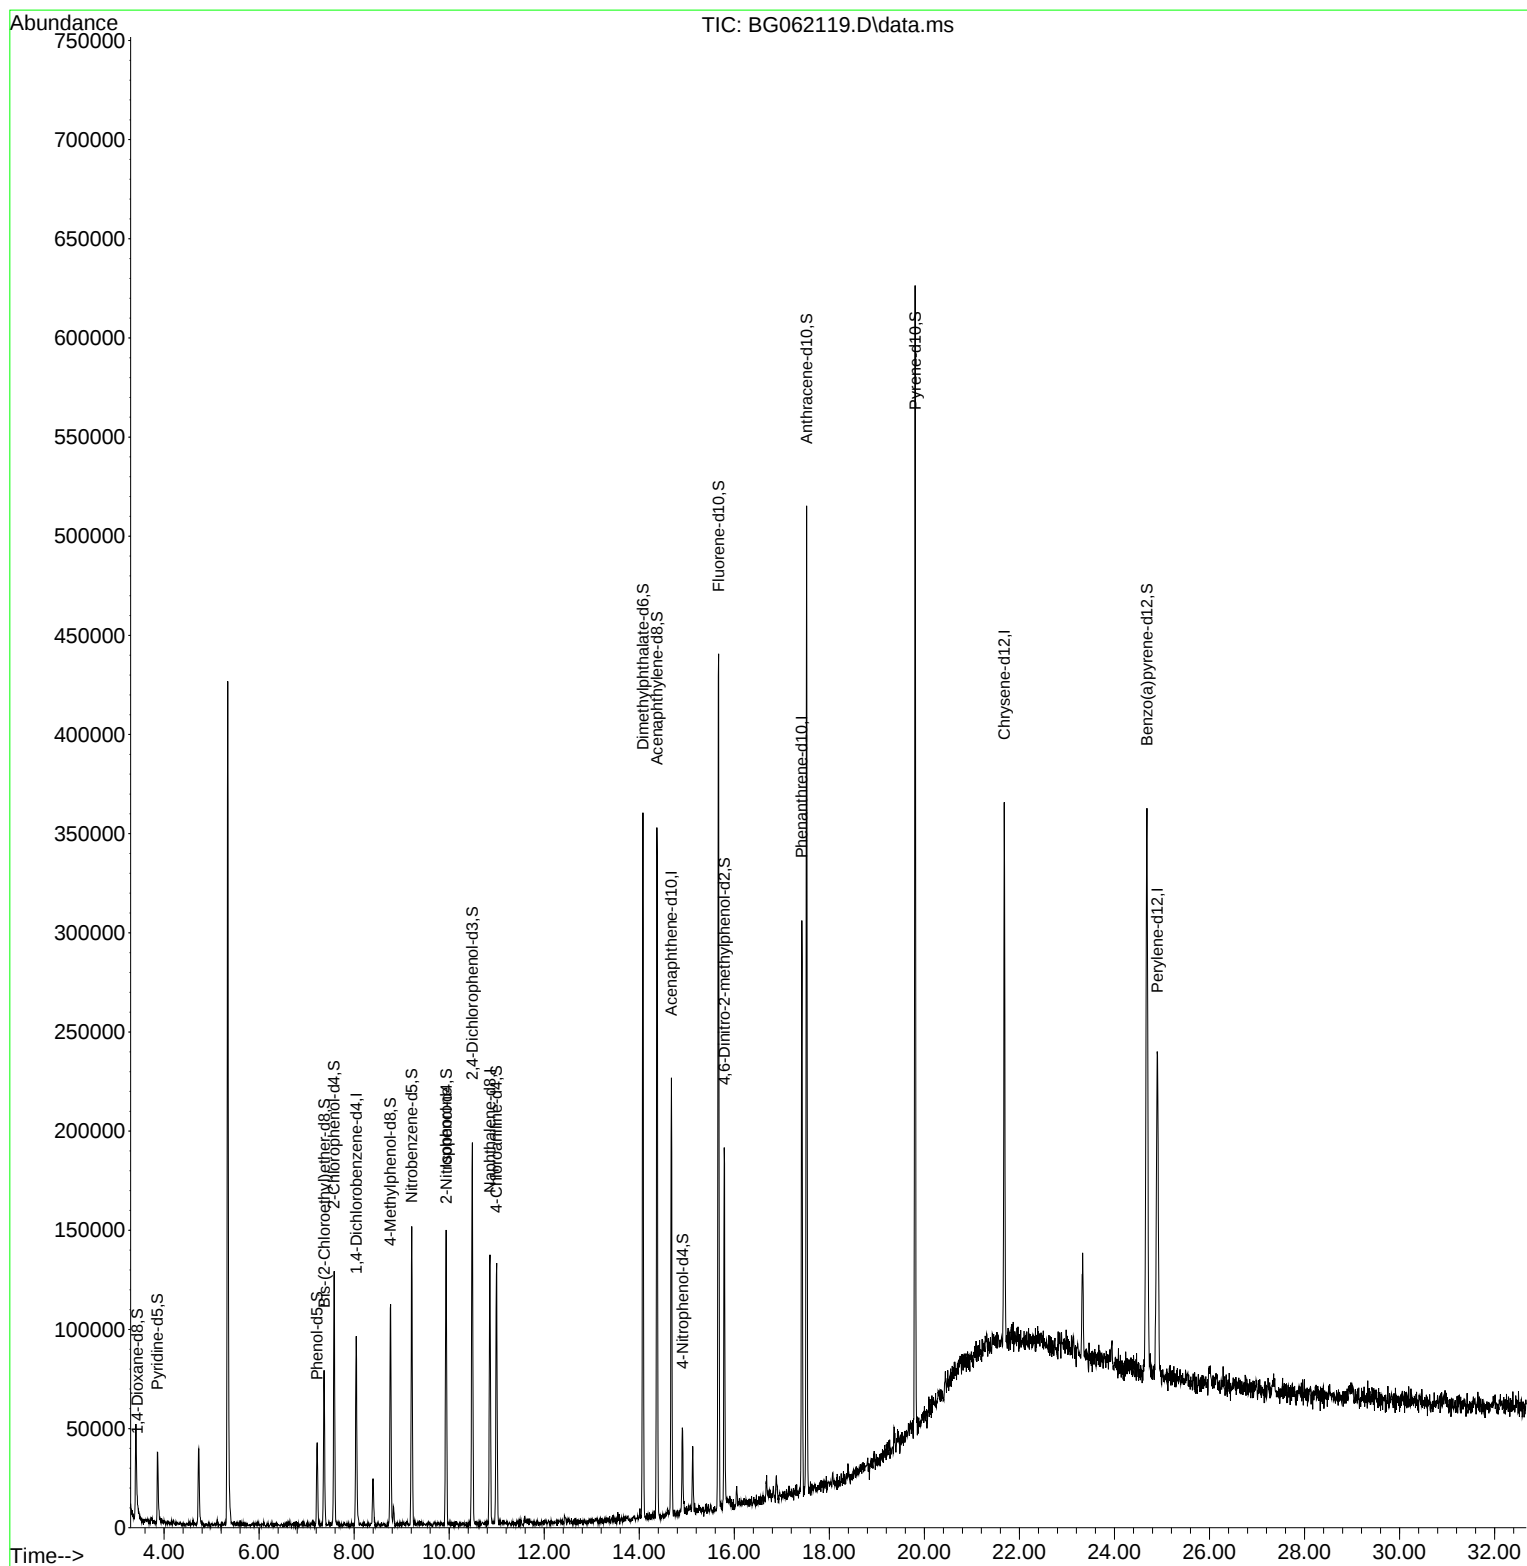

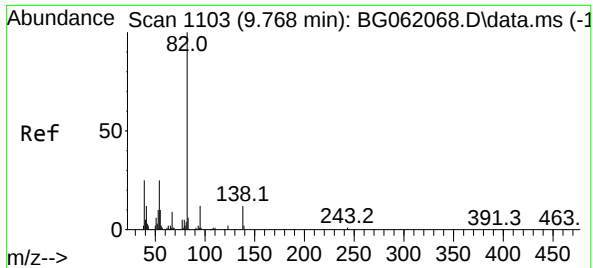

#23
Isophorone
Concen: 1.114 ng/ul
RT: 9.935 min Scan# 11
Delta R.T. 0.160 min
Lab File: BG062119.D
Acq: 17 Jul 2024 19:11

Instrument :
BNA_G
ClientSampleId :
YDZG5

Tgt Ion: 82	Resp:	5498
Ion Ratio	Lower	Upper
82	100	
95	6.3	6.0 9.0
138	0.0	11.9 17.9#

