

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
 Data File : BG062116.D
 Acq On : 17 Jul 2024 17:06
 Operator : MA/JU
 Sample : PB162053BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	12	14	17	rVB	2816	1992	0.25%	0.023%
2	3.405	17	20	23	rBV2	3180	3301	0.42%	0.038%
3	3.441	23	26	29	rVV3	6846	9301	1.18%	0.106%
4	3.529	39	41	45	rVB3	3236	3731	0.47%	0.043%
5	3.658	59	63	64	rBV3	1734	1834	0.23%	0.021%
6	3.705	69	71	72	rBV	2624	2099	0.27%	0.024%
7	3.858	93	97	104	rBV	87226	142311	18.03%	1.626%
8	4.193	152	154	158	rVB2	3146	3751	0.48%	0.043%
9	4.528	210	211	214	rVB	2462	2072	0.26%	0.024%
10	5.691	408	409	413	rVB	2052	1981	0.25%	0.023%
11	5.926	446	449	452	rVV	2256	2321	0.29%	0.027%
12	6.002	460	462	464	rVB	2071	1926	0.24%	0.022%
13	6.678	574	577	579	rBV	1699	2126	0.27%	0.024%
14	6.854	605	607	610	rVB	1681	2105	0.27%	0.024%
15	7.219	661	669	677	rBV2	127454	223904	28.36%	2.558%
16	7.371	687	695	703	rVB	67886	118914	15.06%	1.359%
17	7.436	703	706	708	rBV	2755	2265	0.29%	0.026%
18	7.577	724	730	739	rVV	116599	196580	24.90%	2.246%
19	7.783	761	765	766	rVB	2550	2102	0.27%	0.024%
20	8.041	803	809	817	rVB2	109682	183537	23.25%	2.097%
21	8.364	862	864	870	rBV2	1929	3140	0.40%	0.036%
22	8.541	891	894	899	rBV2	1851	2304	0.29%	0.026%
23	8.764	924	932	942	rBV2	146538	252219	31.95%	2.881%
24	8.870	948	950	954	rVB	1476	1977	0.25%	0.023%
25	8.928	958	960	963	rVV	2222	1910	0.24%	0.022%
26	9.116	989	992	995	rBV	1734	2404	0.30%	0.027%
27	9.210	1001	1008	1015	rBV2	124025	214380	27.16%	2.449%
28	9.604	1073	1075	1078	rVB2	2081	1949	0.25%	0.022%
29	9.939	1123	1132	1142	rVB2	115710	215748	27.33%	2.465%
30	10.045	1147	1150	1154	rVB2	1902	2461	0.31%	0.028%
31	10.139	1160	1166	1168	rBV2	1780	2244	0.28%	0.026%
32	10.168	1168	1171	1172	rBV2	2824	1942	0.25%	0.022%
33	10.485	1217	1225	1232	rVB2	160341	281539	35.67%	3.216%
34	10.767	1272	1273	1276	rBV	2120	1860	0.24%	0.021%
35	10.855	1281	1288	1297	rVB	150999	263806	33.42%	3.014%
36	10.996	1305	1312	1320	rVB2	137837	257722	32.65%	2.944%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
 Data File : BG062116.D
 Acq On : 17 Jul 2024 17:06
 Operator : MA/JU
 Sample : PB162053BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

37	11.578	1406	1411	1413	rBV2	2616	2786	0.35%	0.032%
38	11.725	1435	1436	1440	rVB2	2510	2254	0.29%	0.026%
39	11.796	1443	1448	1449	rVV2	1666	2391	0.30%	0.027%
40	12.078	1493	1496	1499	rVV2	2291	2139	0.27%	0.024%
41	12.430	1554	1556	1562	rVB2	2730	3555	0.45%	0.041%
42	12.788	1615	1617	1620	rBV2	1591	1837	0.23%	0.021%
43	13.223	1688	1691	1693	rBV2	1693	2071	0.26%	0.024%
44	13.452	1728	1730	1732	rBV2	2125	1980	0.25%	0.023%
45	14.075	1829	1836	1845	rVB	310118	442498	56.06%	5.055%
46	14.375	1877	1887	1893	rBV2	286612	456686	57.85%	5.217%
47	14.539	1912	1915	1919	rBV2	1943	2912	0.37%	0.033%
48	14.675	1930	1938	1944	rBV	246439	378983	48.01%	4.330%
49	14.816	1960	1962	1966	rBV	2386	2537	0.32%	0.029%
50	14.904	1970	1977	1987	rBV	143642	248849	31.52%	2.843%
51	15.268	2035	2039	2042	rVB	2243	2711	0.34%	0.031%
52	15.667	2099	2107	2116	rVB	380626	568120	71.97%	6.490%
53	15.791	2122	2128	2135	rBV	158801	242206	30.68%	2.767%
54	15.838	2135	2136	2141	rVV2	3899	4464	0.57%	0.051%
55	15.891	2144	2145	2146	rBV2	4462	1889	0.24%	0.022%
56	15.979	2158	2160	2165	rBV2	2355	3445	0.44%	0.039%
57	16.120	2183	2184	2188	rBV2	4118	4205	0.53%	0.048%
58	16.373	2226	2227	2231	rVB	3360	2695	0.34%	0.031%
59	16.443	2237	2239	2243	rVB2	4639	4450	0.56%	0.051%
60	16.555	2255	2258	2259	rVV2	2781	1939	0.25%	0.022%
61	16.602	2263	2266	2268	rVB	2451	2429	0.31%	0.028%
62	16.643	2268	2273	2275	rBV	2677	3430	0.43%	0.039%
63	16.678	2277	2279	2283	rVB2	3022	4126	0.52%	0.047%
64	16.725	2285	2287	2290	rVB	2422	2119	0.27%	0.024%
65	16.760	2290	2293	2294	rBV	2567	2597	0.33%	0.030%
66	16.854	2305	2309	2311	rBV	1802	2418	0.31%	0.028%
67	16.878	2311	2313	2318	rVB	2324	3229	0.41%	0.037%
68	16.925	2318	2321	2322	rBV	2007	1842	0.23%	0.021%
69	16.972	2327	2329	2330	rVB	3525	2140	0.27%	0.024%
70	16.984	2330	2331	2333	rBV	2743	2290	0.29%	0.026%
71	17.301	2383	2385	2387	rVB	2413	2123	0.27%	0.024%
72	17.342	2391	2392	2394	rVV	2717	1963	0.25%	0.022%
73	17.424	2399	2406	2412	rBV	338401	509511	64.54%	5.821%
74	17.518	2416	2422	2429	rBV	437359	675596	85.58%	7.718%
75	17.612	2437	2438	2440	rBV	2838	2175	0.28%	0.025%
76	17.700	2450	2453	2456	rBV2	2174	3497	0.44%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
 Data File : BG062116.D
 Acq On : 17 Jul 2024 17:06
 Operator : MA/JU
 Sample : PB162053BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
 Title : SVOA CALIBRATION

77	17.724	2456	2457	2460	rVB2	2726	2050	0.26%	0.023%
78	17.836	2472	2476	2477	rBV3	3816	4801	0.61%	0.055%
79	17.847	2477	2478	2480	rBV	2577	2116	0.27%	0.024%
80	17.959	2494	2497	2500	rBV2	3426	4815	0.61%	0.055%
81	18.053	2510	2513	2514	rBV2	3280	2576	0.33%	0.029%
82	18.065	2514	2515	2518	rBV	4481	3374	0.43%	0.039%
83	18.206	2537	2539	2540	rBV2	2058	2130	0.27%	0.024%
84	18.217	2540	2541	2545	rVV2	5048	3751	0.48%	0.043%
85	18.259	2547	2548	2551	rVB3	3183	2468	0.31%	0.028%
86	18.317	2557	2558	2561	rVB3	3312	2278	0.29%	0.026%
87	18.341	2561	2562	2564	rBV	3210	2465	0.31%	0.028%
88	18.388	2569	2570	2572	rBV	3034	2029	0.26%	0.023%
89	18.682	2618	2620	2621	rBV2	4135	2912	0.37%	0.033%
90	18.781	2635	2637	2638	rBV2	4656	2400	0.30%	0.027%
91	18.840	2645	2647	2649	rVB2	7001	4932	0.62%	0.056%
92	18.870	2649	2652	2653	rBV3	5159	5798	0.73%	0.066%
93	19.099	2689	2691	2692	rBV2	4180	1931	0.24%	0.022%
94	19.116	2692	2694	2695	rBV2	3876	3077	0.39%	0.035%
95	19.363	2733	2736	2741	rBV6	8393	13371	1.69%	0.153%
96	19.440	2747	2749	2752	rVB4	6568	5022	0.64%	0.057%
97	19.804	2805	2811	2817	rVB2	541610	767704	97.25%	8.771%
98	21.684	3125	3131	3139	rVB	320588	517756	65.59%	5.915%
99	24.680	3633	3641	3654	rVB3	277412	789390	100.00%	9.018%
100	24.904	3671	3679	3691	rVB2	206034	579177	73.37%	6.617%




Sum of corrected areas: 8753168

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
Data File : BG062116.D
Acq On : 17 Jul 2024 17:06
Operator : MA/JU
Sample : PB162053BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

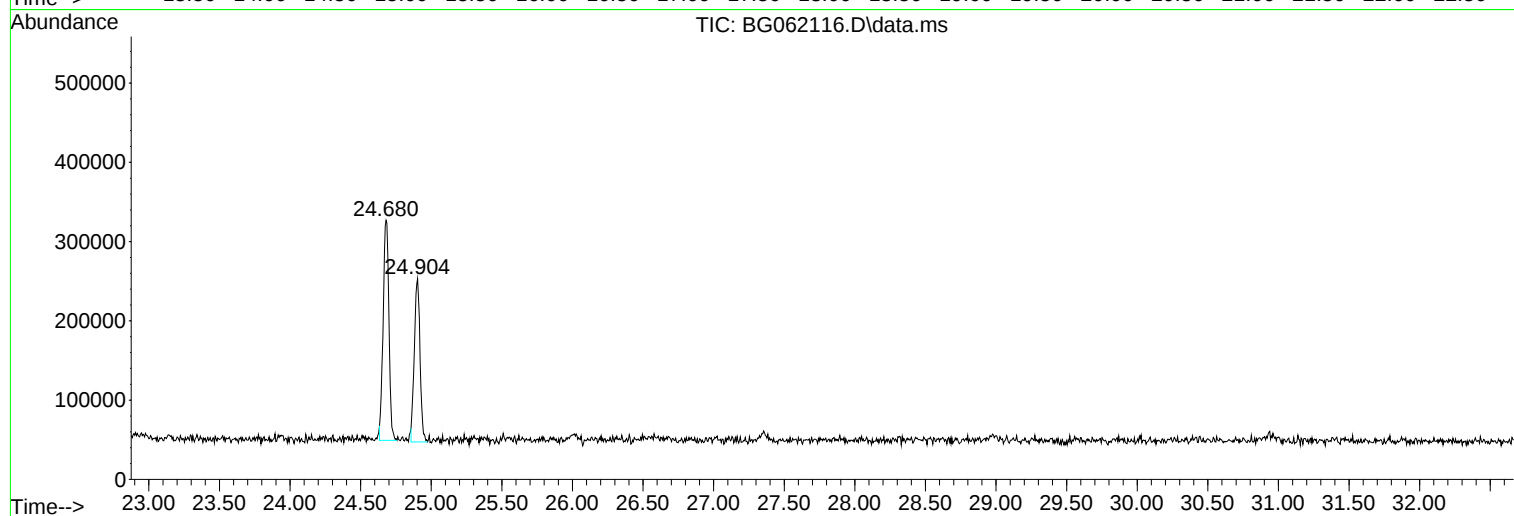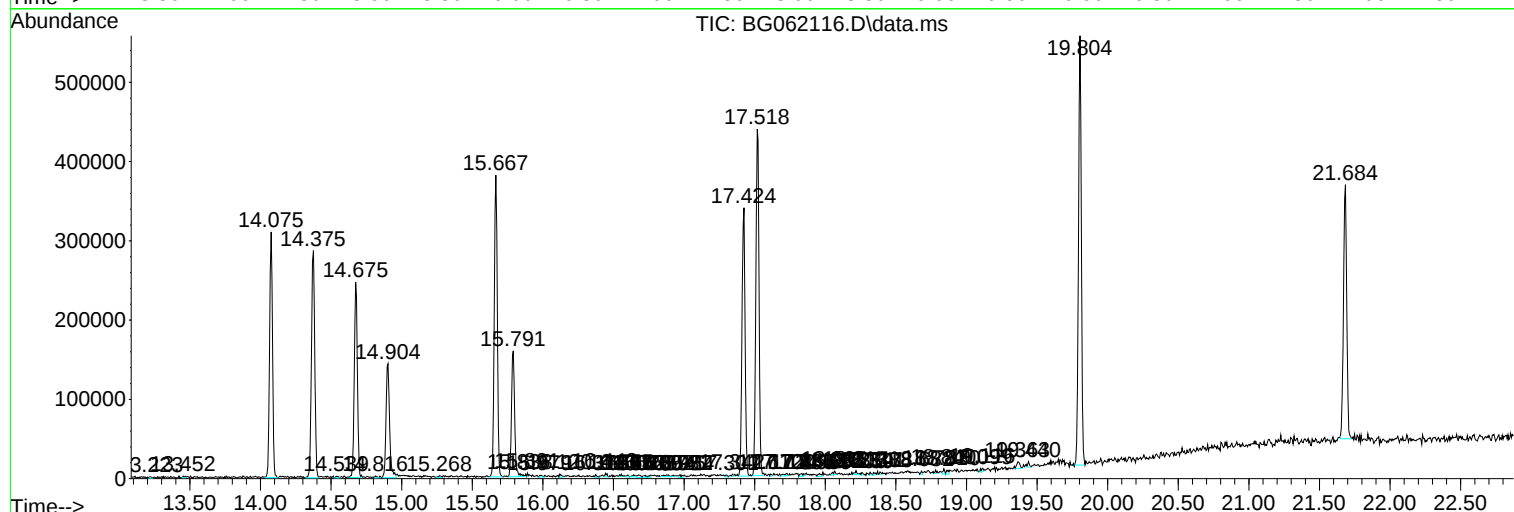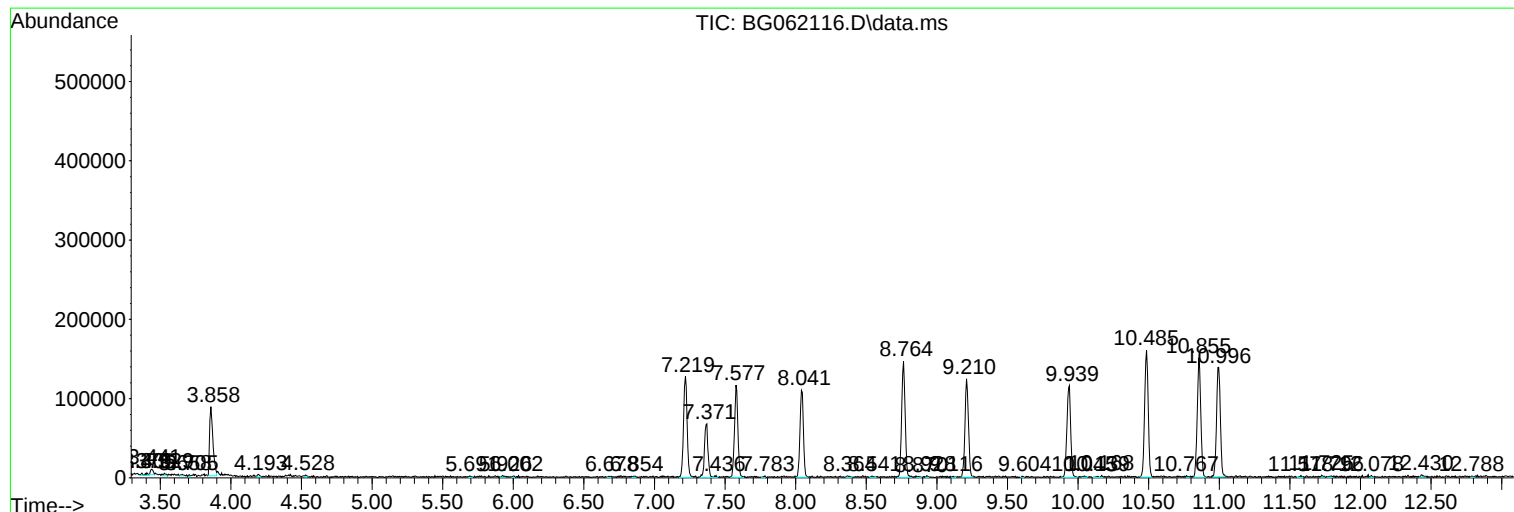

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
Data File : BG062116.D
Acq On : 17 Jul 2024 17:06
Operator : MA/JU
Sample : PB162053BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071724\
Data File : BG062116.D
Acq On : 17 Jul 2024 17:06
Operator : MA/JU
Sample : PB162053BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG070224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc