
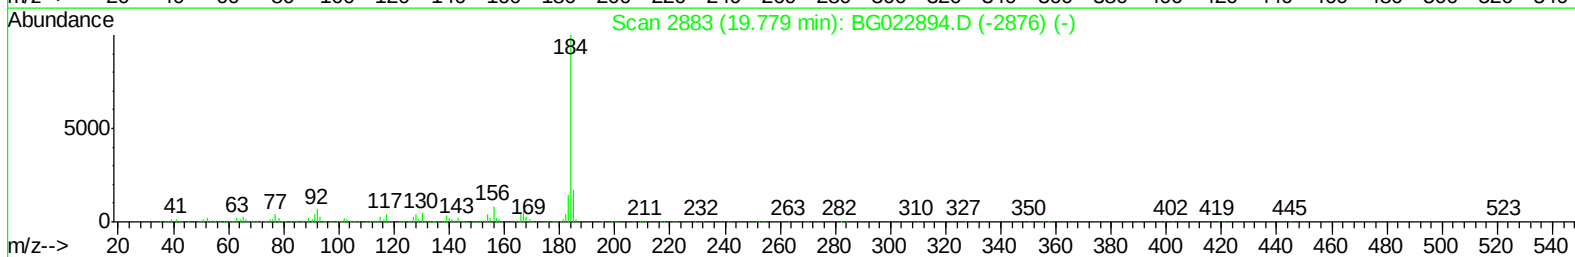
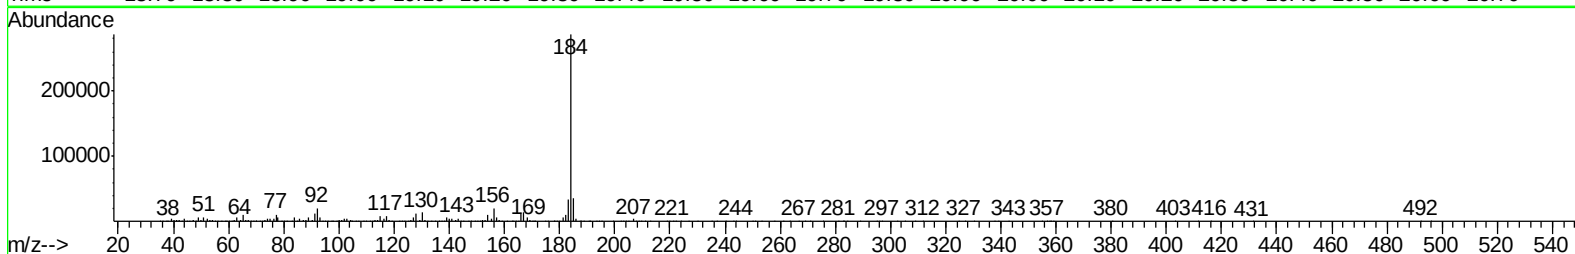


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071816\
Data File : BG023156.D
Acq On : 18 Jul 2016 10:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 07:01:29 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 01:16:03 2016
Response via : Initial Calibration

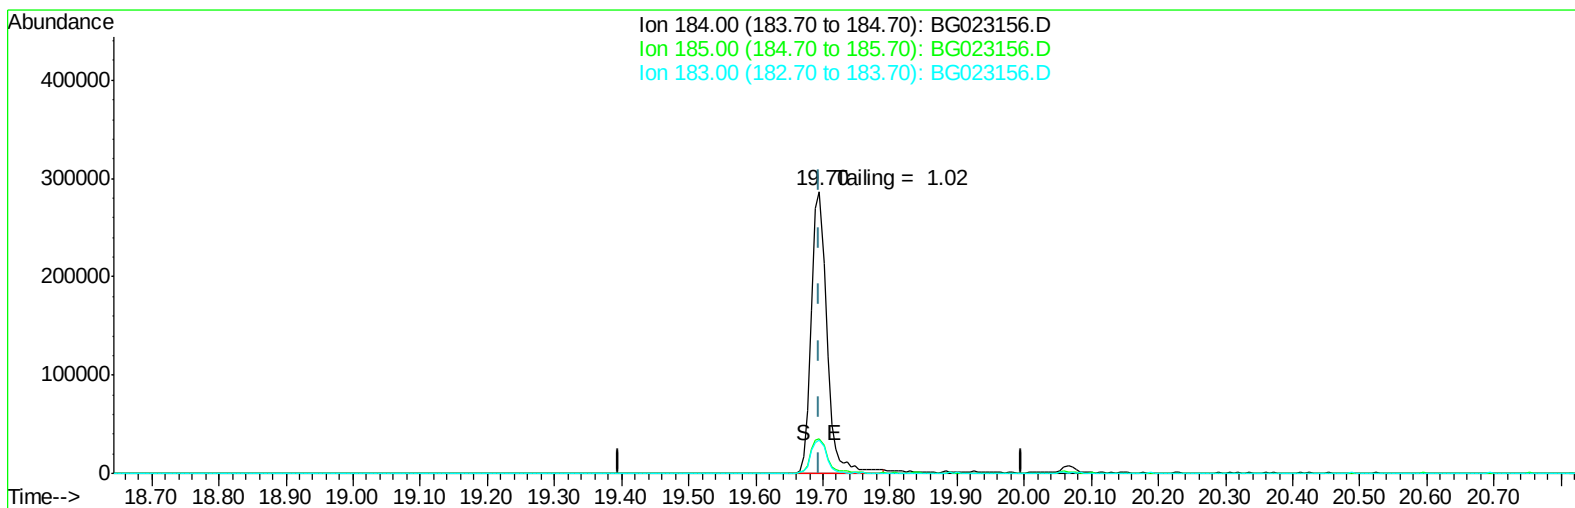

TIC: BG023156.D

(76) Benzidine




19.695min (-0.001) 317.52ng

response 460612

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	12.37#
183.00	13.40	11.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG071816\
Data File : BG023156.D
Acq On : 18 Jul 2016 10:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 07:01:29 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 01:16:03 2016
Response via : Initial Calibration

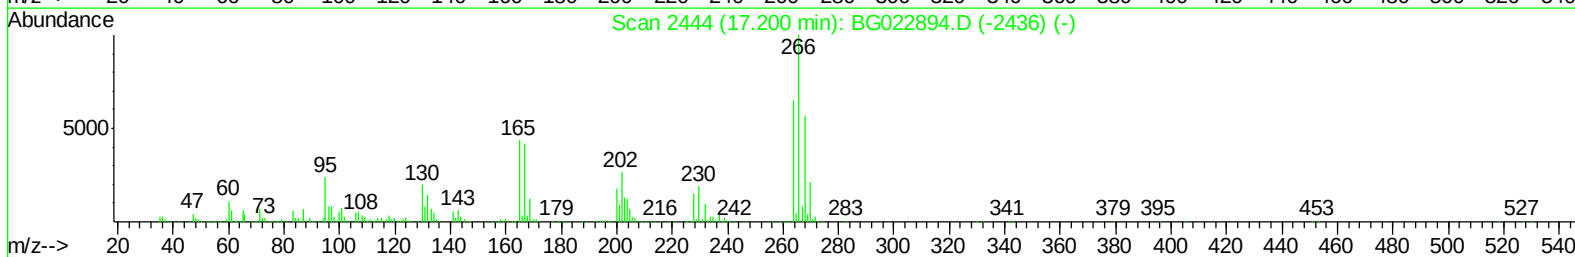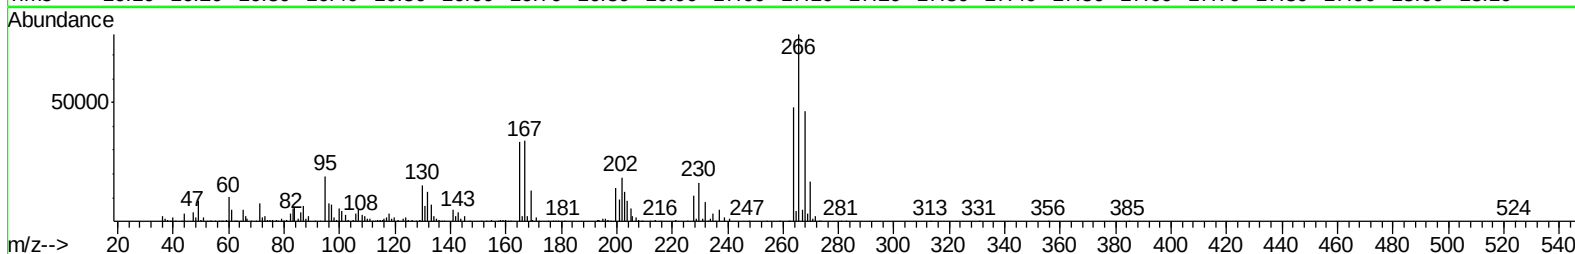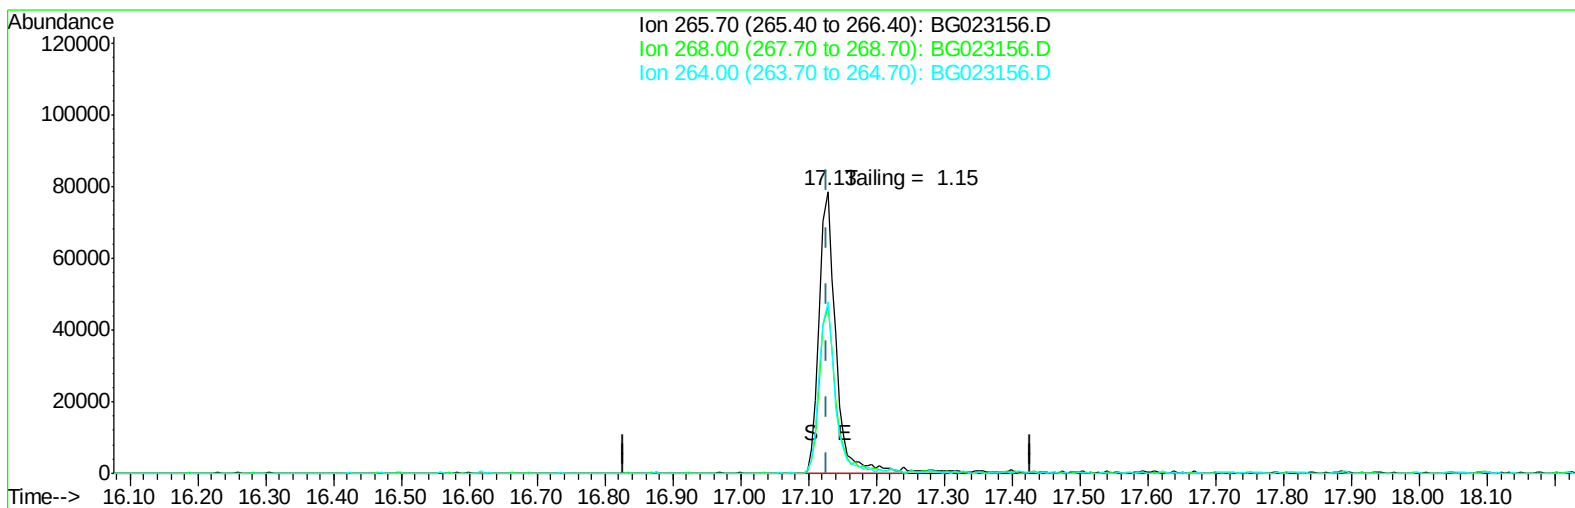

TIC: BG023156.D

(69) Pentachlorophenol (C)

17.128min (-0.001) 103771.80ng

response 132140

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.33
264.00	63.20	60.98
0.00	0.00	0.00