


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG071816\
 Data File : BG023156.D
 Acq On : 18 Jul 2016 10:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 01:16:03 2016

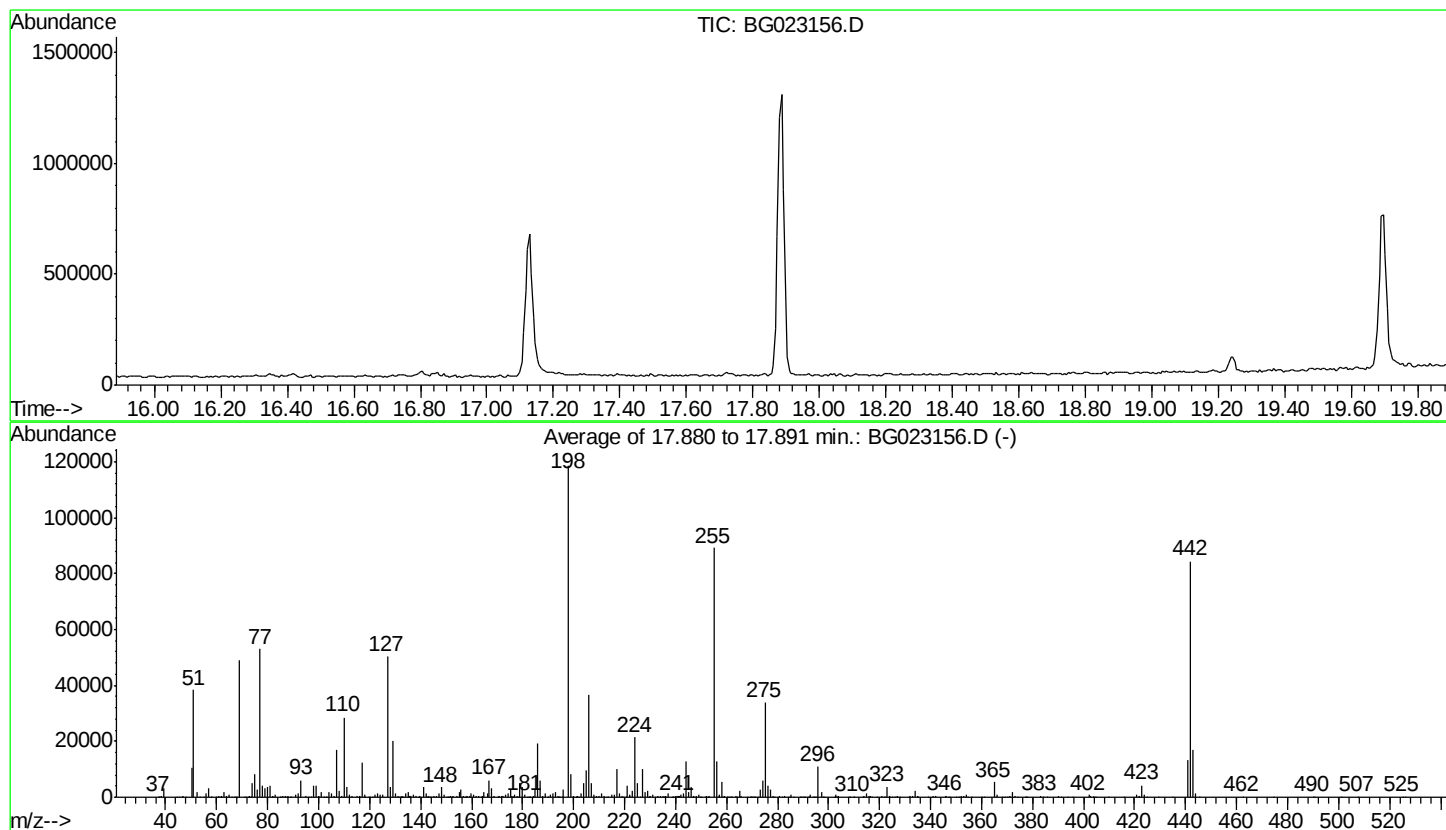

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	38380	PASS
68	69	0.00	2	0.2	104	PASS
69	198	0.00	100	41.2	48833	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	50314	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118610	PASS
199	198	5	9	7.1	8458	PASS
275	198	10	60	28.5	33848	PASS
365	198	1	100	4.5	5340	PASS
441	442	0.01	24	15.7	13230	PASS
442	198	50	100	71.2	84477	PASS
443	442	15	24	19.8	16757	PASS