
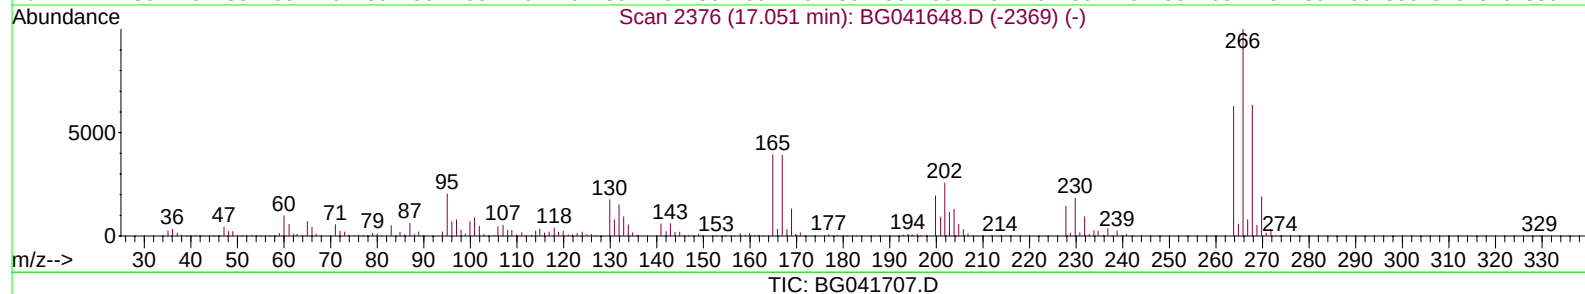
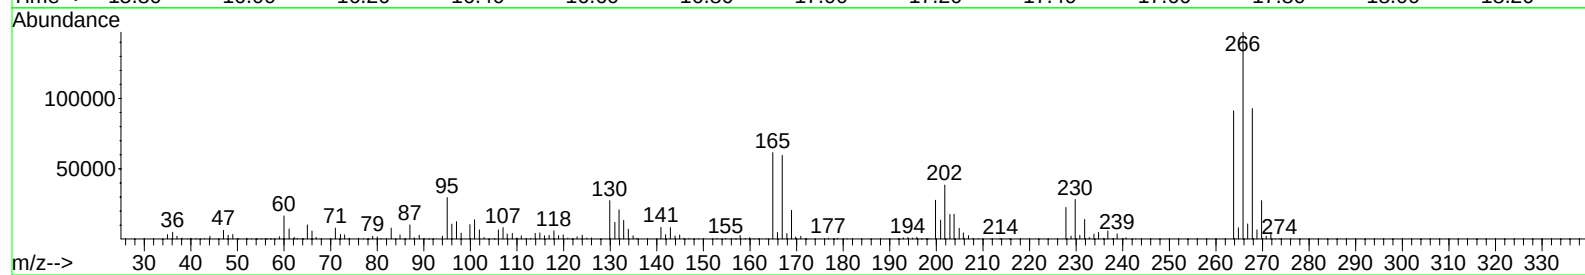


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071819\
Data File : BG041707.D
Acq On : 18 Jul 2019 11:48
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 18:15:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

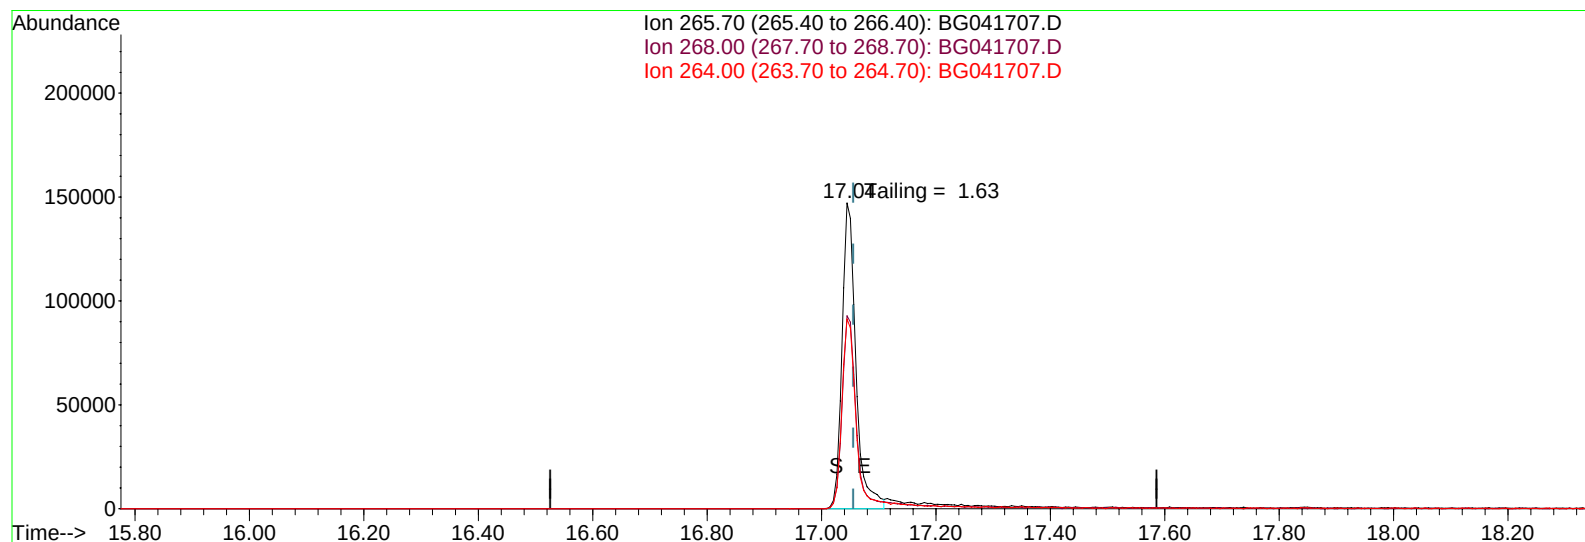

(70) Pentachlorophenol (C)




17.044min (-0.011) 621505.18ng

response 256091

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.11
264.00	64.30	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071819\
Data File : BG041707.D
Acq On : 18 Jul 2019 11:48
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 18 18:15:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

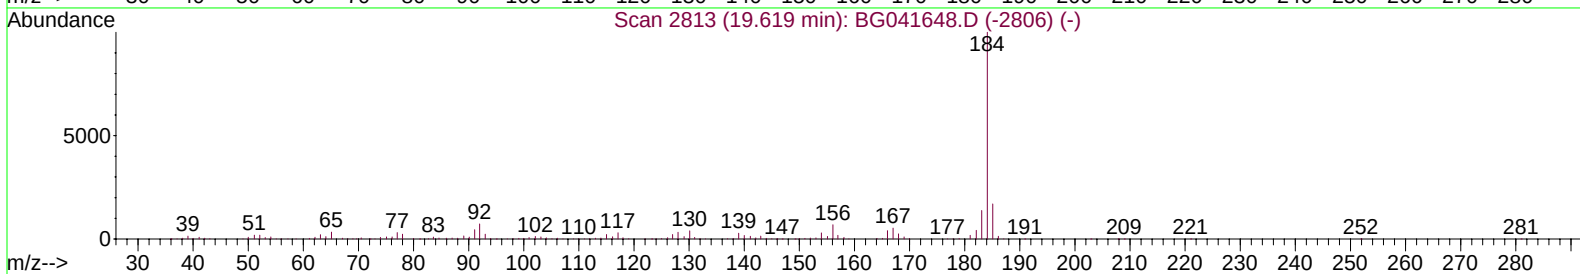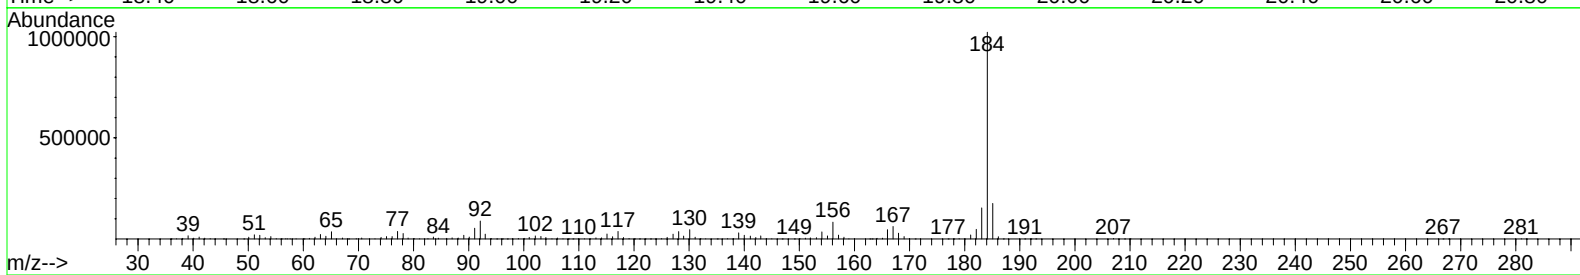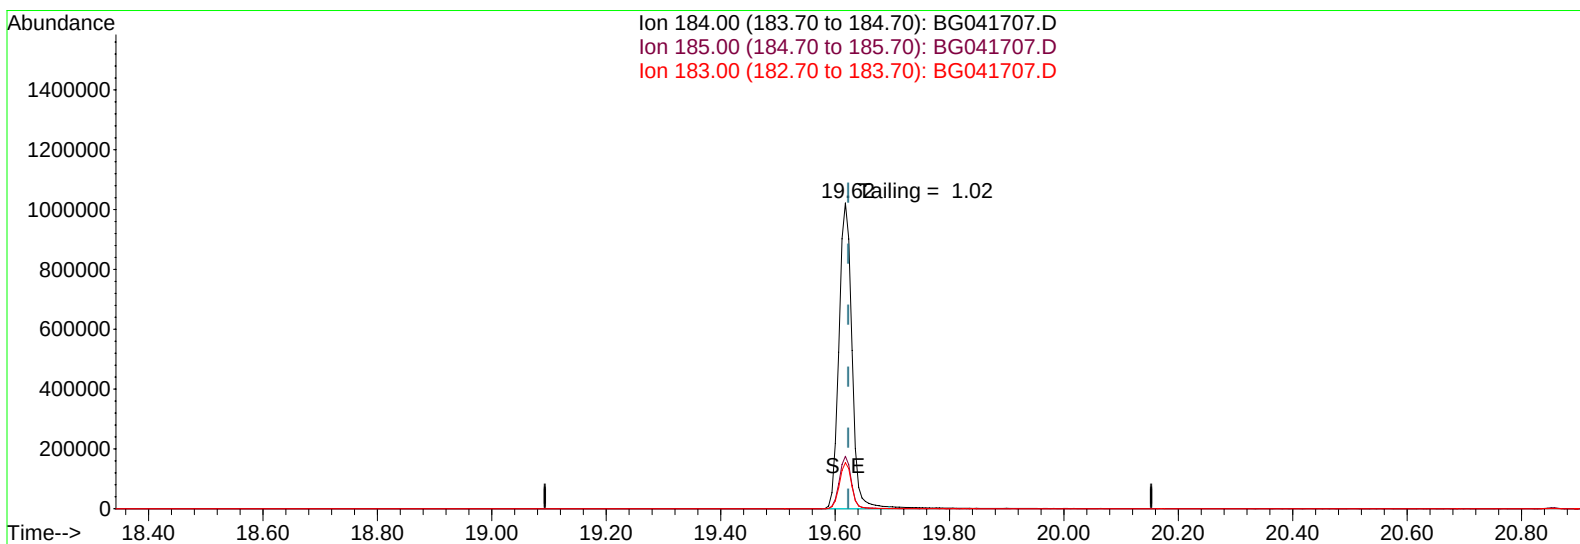

TIC: BG041707.D

(77) Benzidine

19.618min (-0.005) -20.00ng

response 1636352

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	17.17
183.00	14.70	15.05
0.00	0.00	0.00