


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071819\  
 Data File : BG041707.D  
 Acq On : 18 Jul 2019 11:48  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG071519.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jul 15 16:16:21 2019

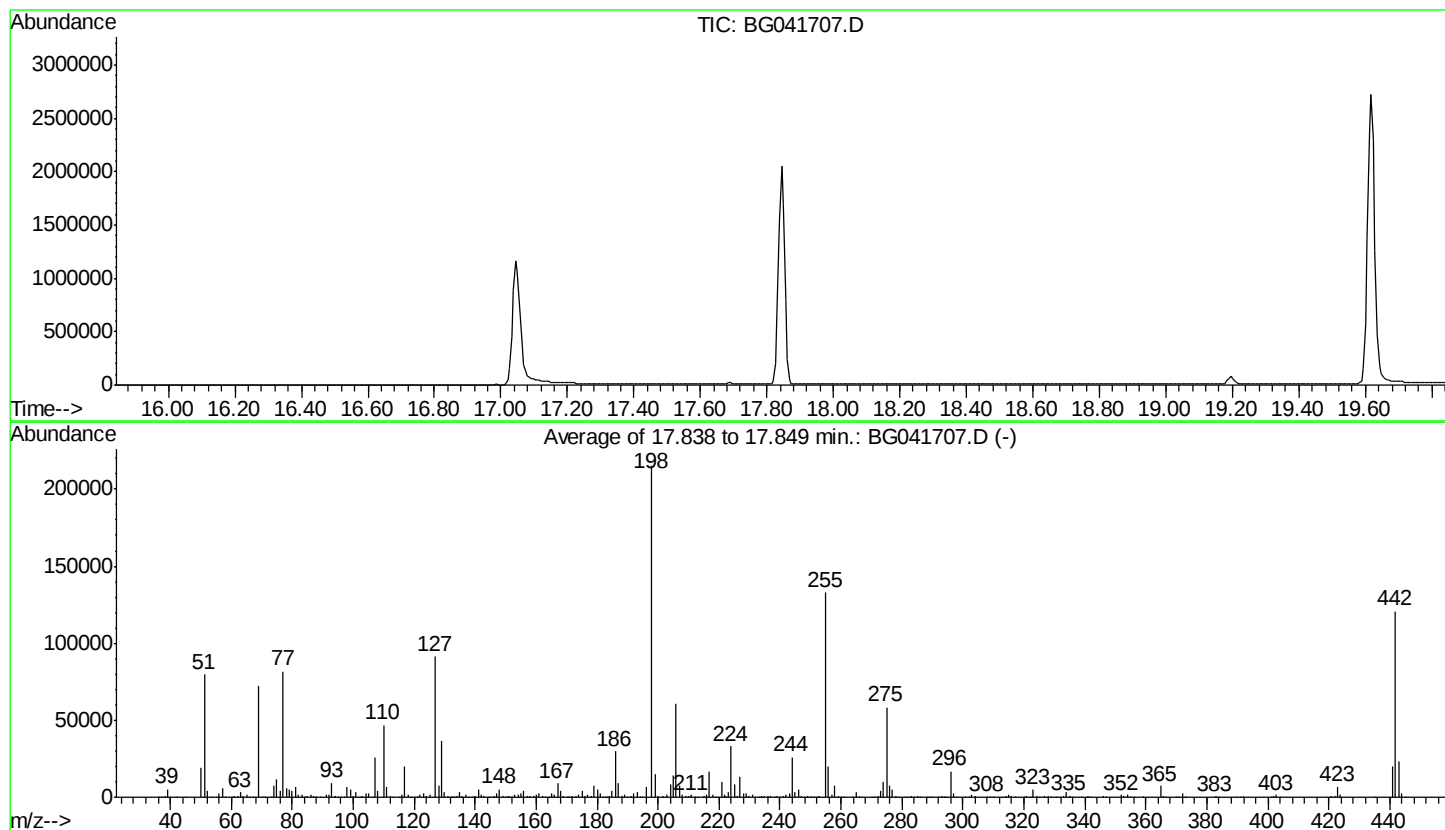

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.9      | 79522   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 33.7      | 72613   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 408     | PASS             |
| 127         | 198          | 10           | 80           | 42.3      | 91122   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 215296  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 14923   | PASS             |
| 275         | 198          | 10           | 60           | 27.1      | 58400   | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 7409    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.2       | 19788   | PASS             |
| 442         | 198          | 50           | 100          | 56.1      | 120762  | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 23710   | PASS             |