


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071822\  
 Data File : BG054307.D  
 Acq On : 18 Jul 2022 9:47  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 15 15:54:11 2022

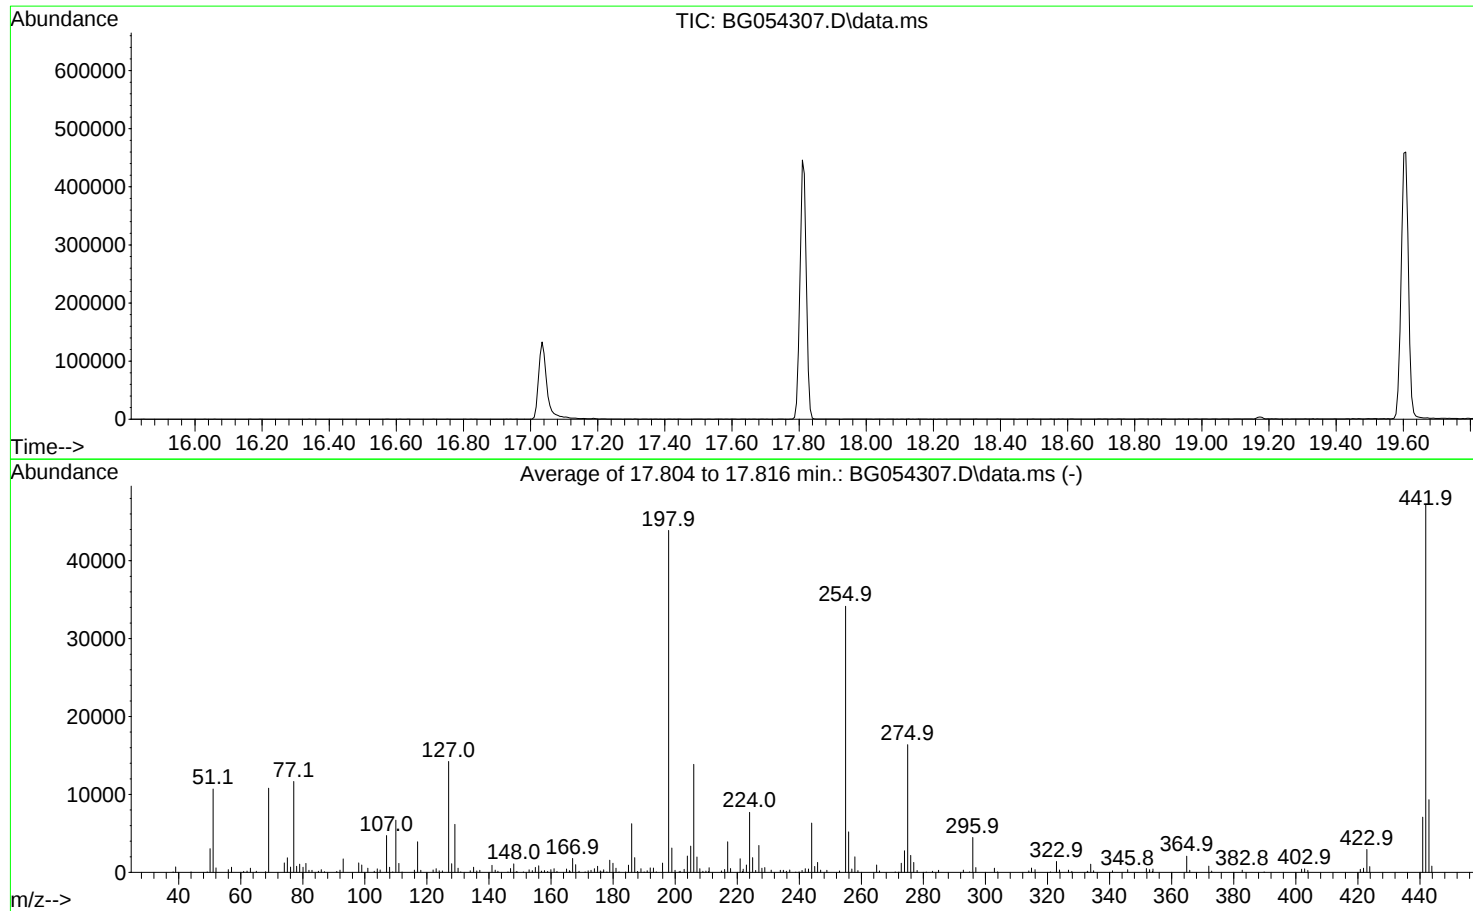




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 24.4         | 10704      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.8          | 91         | PASS                |
| 69             | 198             | 0.00            | 100             | 24.6         | 10804      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 32.4         | 14237      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 43883      | PASS                |
| 199            | 198             | 5               | 9               | 7.1          | 3131       | PASS                |
| 275            | 198             | 10              | 60              | 37.3         | 16385      | PASS                |
| 365            | 198             | 1               | 100             | 4.7          | 2067       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.1         | 7081       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 47211      | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 9322       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071822\  
Data File : BG054307.D  
Acq On : 18 Jul 2022 9:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jul 18 16:14:34 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 15 15:54:11 2022  
Response via : Initial Calibration

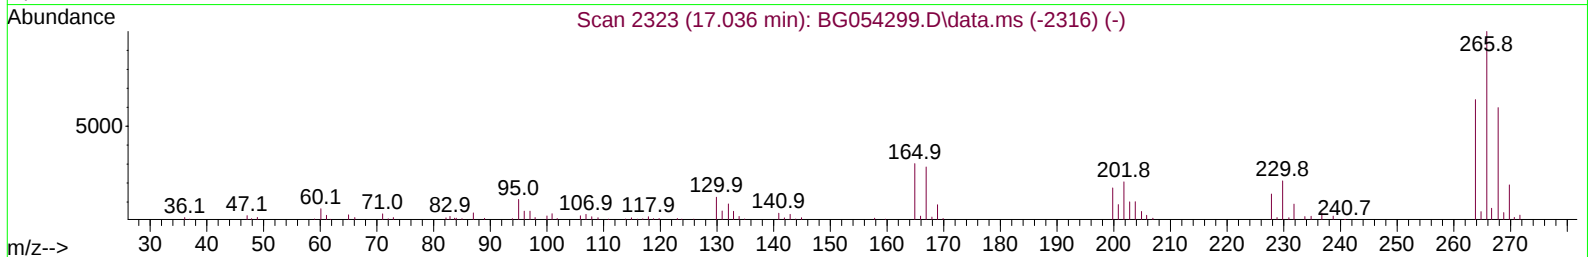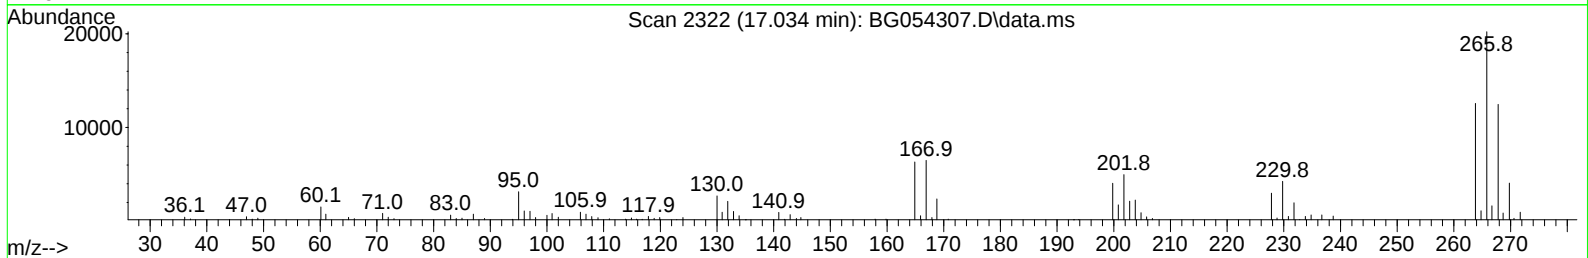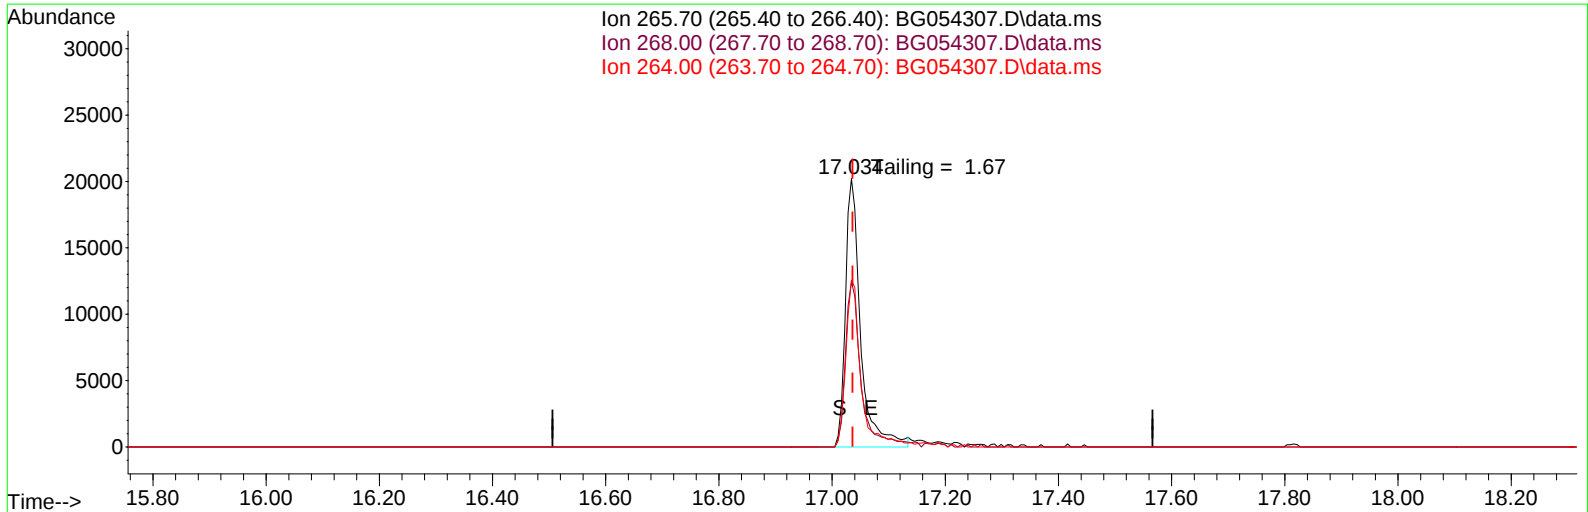

TIC: BG054307.D\data.ms

**(70) Pentachlorophenol (C)**

17.034min (-0.002) 39841.34 ng




response 37285

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 70.20  | 65.96  |
| 264.00 | 66.20  | 62.19  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071822\  
 Data File : BG054307.D  
 Acq On : 18 Jul 2022 9:47  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Jul 18 16:14:34 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jul 15 15:54:11 2022  
 Response via : Initial Calibration

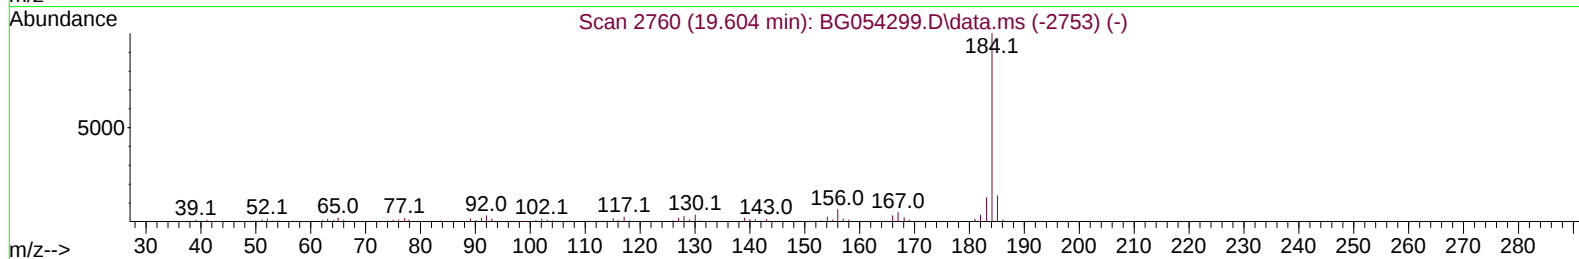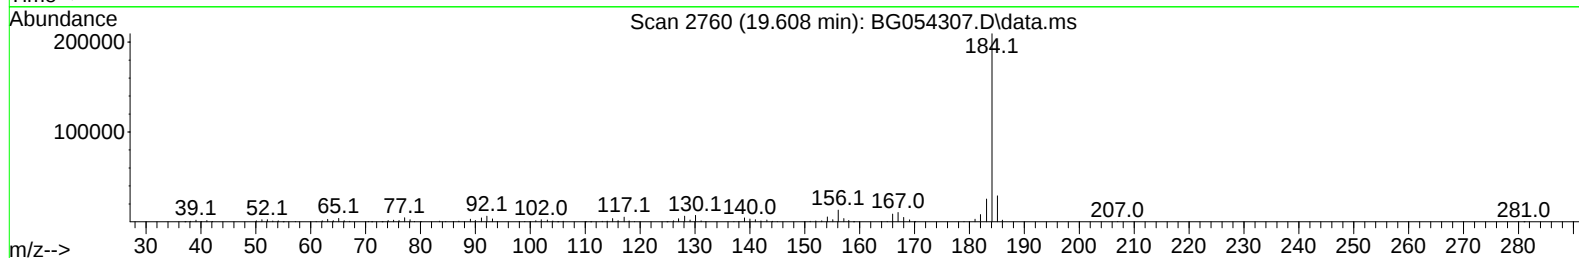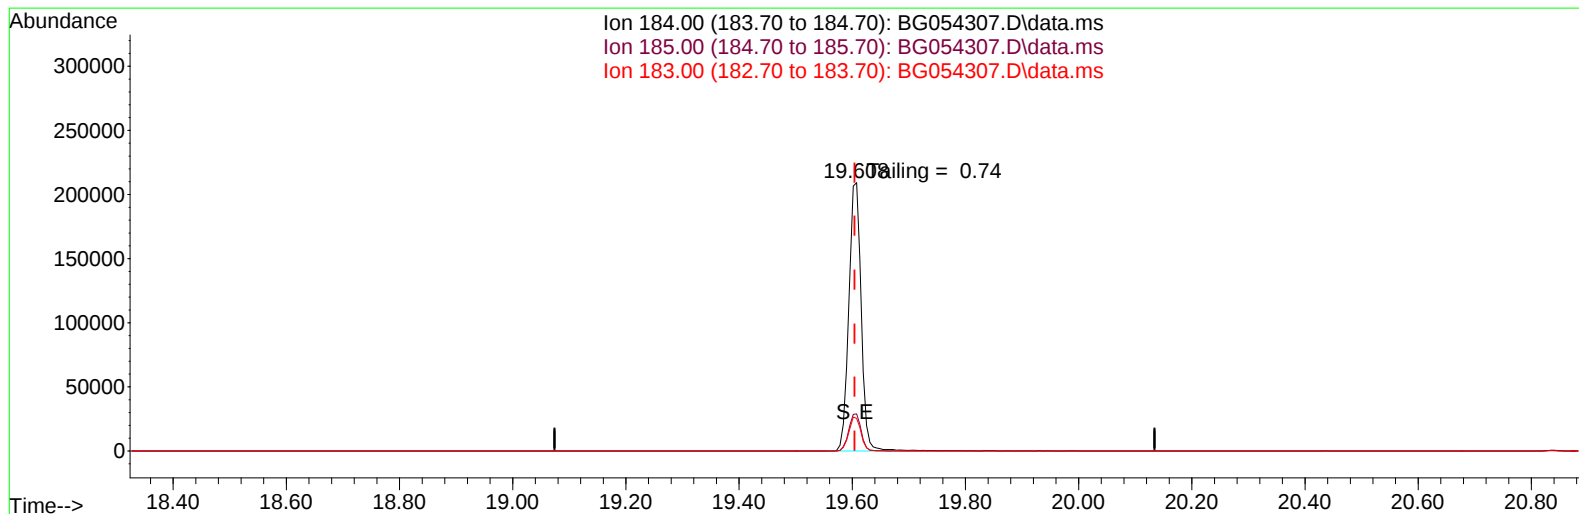

TIC: BG054307.D\data.ms

**(77) Benzidine**

19.608min (+ 0.004) 0.00 ng

response 318542

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 13.85  |
| 183.00 | 11.10  | 12.17  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/18/2022     | BNA_G            | <u>BG054307.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 194094           | 20.83              |
| DDD           | 1651             | 20.39              |
| DDE           | 0                | 19.9               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 1651          | 195745           | 0.84               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP