


Data Path : Z:\HPCHEM1\BNA_G\Data\BG071915\
 Data File : BG017964.D
 Acq On : 19 Jul 2015 18:48
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

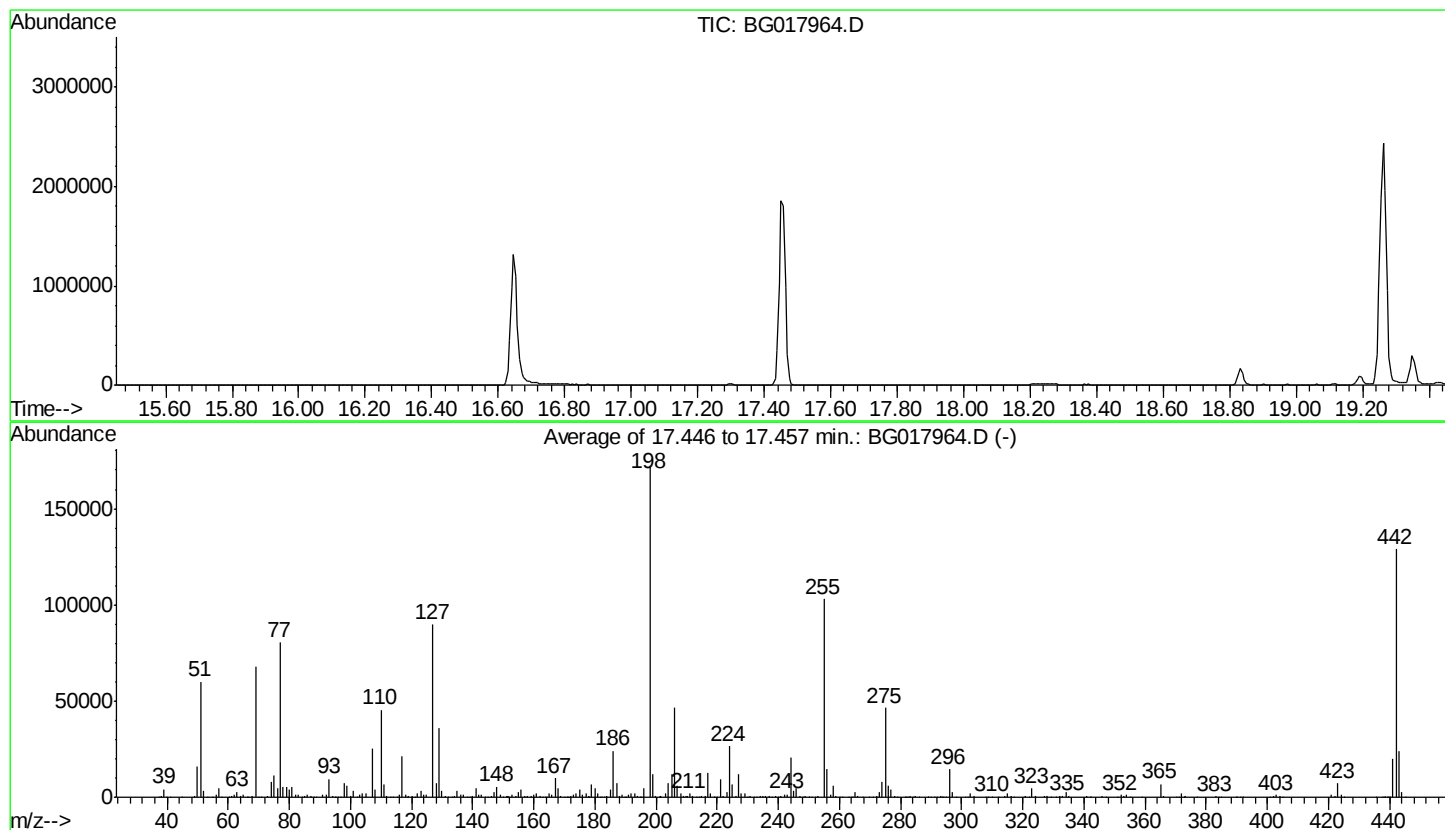

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	59991	PASS
68	69	0.00	2	0.6	399	PASS
69	198	0.00	100	39.4	67952	PASS
70	69	0.00	2	0.5	317	PASS
127	198	10	80	52.1	89706	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	172325	PASS
199	198	5	9	6.8	11725	PASS
275	198	10	60	26.9	46309	PASS
365	198	1	100	3.9	6732	PASS
441	442	0.01	24	15.3	19711	PASS
442	198	50	100	74.9	129002	PASS
443	442	15	24	18.8	24284	PASS