


Data Path : Z:\HPCHEM1\BNA G\DATA\BG071916\
 Data File : BG023171.D
 Acq On : 19 Jul 2016 10:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG070816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 19 15:46:37 2016

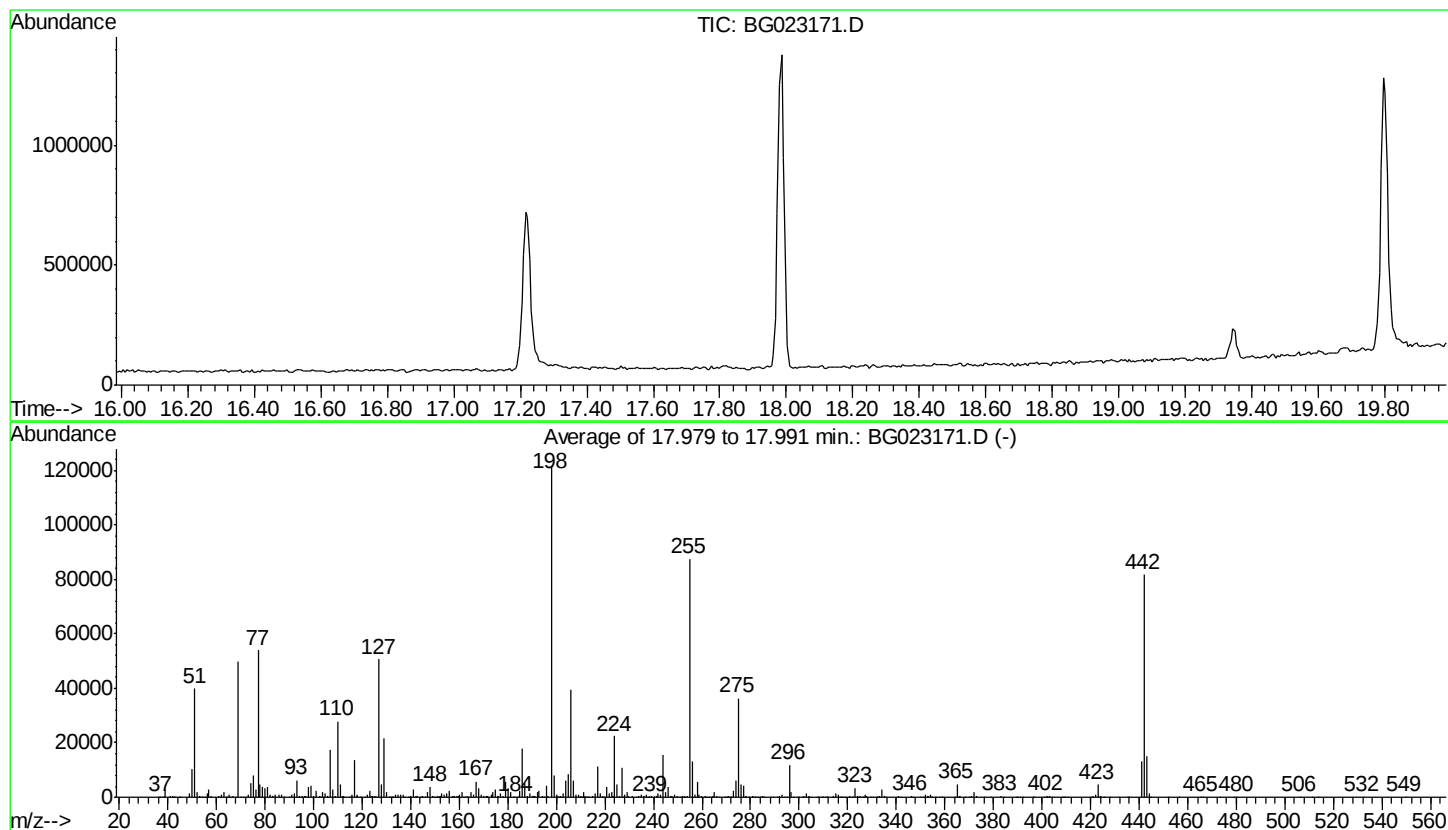

AutoFind: Scans 2577, 2578, 2579; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	39786	PASS
68	69	0.00	2	0.2	116	PASS
69	198	0.00	100	40.9	49756	PASS
70	69	0.00	2	0.3	154	PASS
127	198	10	80	41.5	50597	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121778	PASS
199	198	5	9	6.8	8232	PASS
275	198	10	60	29.8	36349	PASS
365	198	1	100	4.0	4883	PASS
441	442	0.01	24	16.2	13219	PASS
442	198	50	100	67.0	81602	PASS
443	442	15	24	18.4	14974	PASS