

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027963.D
 Acq On : 19 Jul 2017 15:37
 Operator : SJ/JU
 Sample : PB100701BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Quant Time: Jul 20 04:53:53 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 02:43:07 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	43080	20.00	ng/ul	0.00
18) Naphthalene-d8	11.20	136	184020	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	129359	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.73	188	338603	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	396126	20.00	ng/ul	0.00
83) Perylene-d12	25.58	264	374703	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.87	96	6514	8.33	ng/uL	0.00
5) Phenol-d5	7.52	99	125053	35.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.70	67	75536	37.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.92	132	104430	37.55	ng/ul	0.00
13) 4-Methylphenol-d8	9.07	113	102412	34.95	ng/ul	0.00
19) Nitrobenzene-d5	9.55	128	48228	35.62	ng/ul	0.00
22) 2-Nitrophenol-d4	10.27	143	59341	36.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.82	165	109984	34.51	ng/ul	0.00
29) 4-Chloroaniline-d4	11.33	131	141158	48.99	ng/ul	0.00
43) Dimethylphthalate-d6	14.38	166	429954	38.34	ng/ul	0.00
46) Acenaphthylene-d8	14.68	160	445486	34.95	ng/ul	0.00
51) 4-Nitrophenol-d4	15.17	143	46169	28.43	ng/ul	0.00
57) Fluorene-d10	15.97	176	378029	35.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.08	200	67225	28.58	ng/ul	0.00
70) Anthracene-d10	17.83	188	632171	38.72	ng/ul	0.00
76) Pyrene-d10	20.10	212	724903	40.73	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.34	264	679196	38.81	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.08	70	2631	1.242	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027963.D
Acq On : 19 Jul 2017 15:37
Operator : SJ/JU
Sample : PB100701BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Quant Time: Jul 20 04:53:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 02:43:07 2017
Response via : Initial Calibration

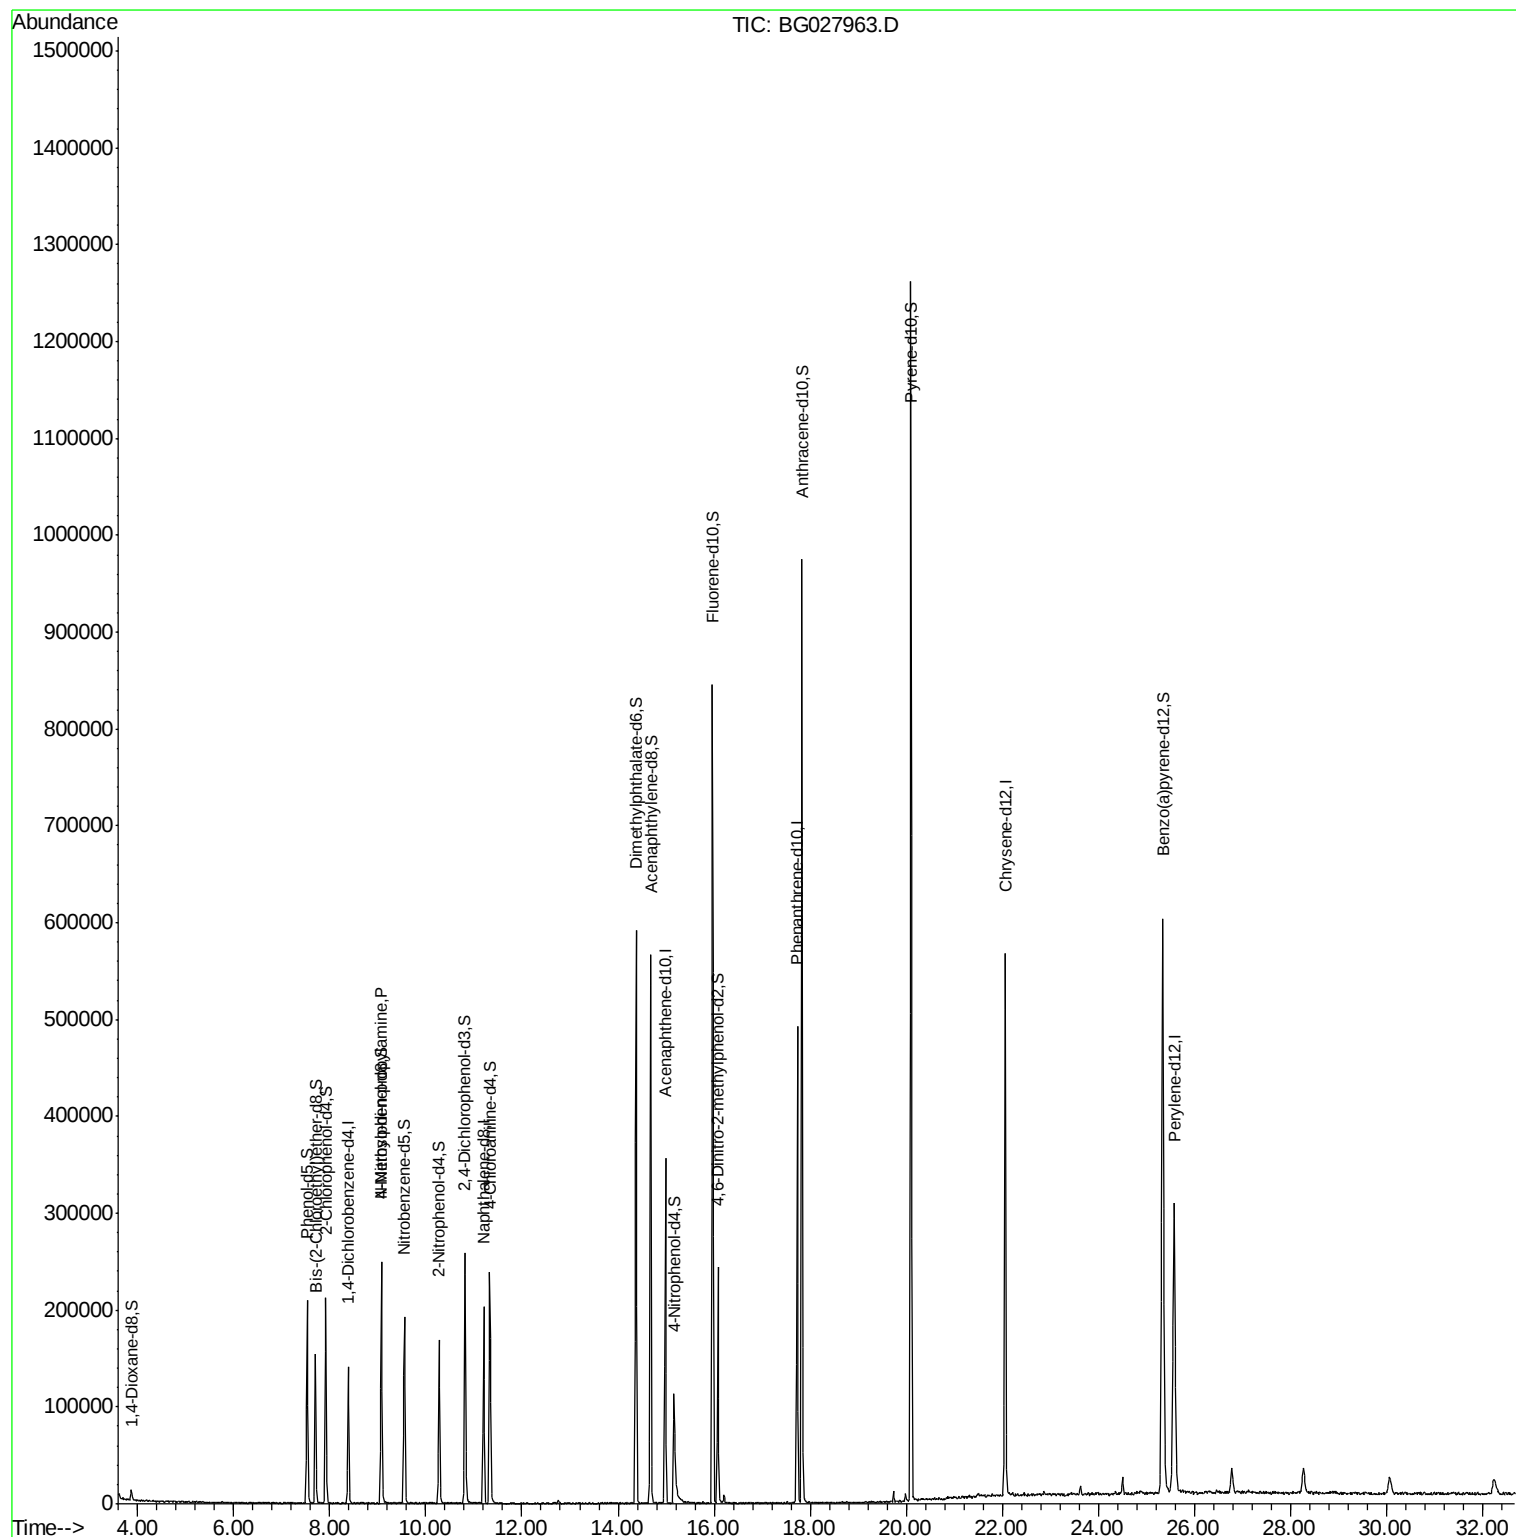

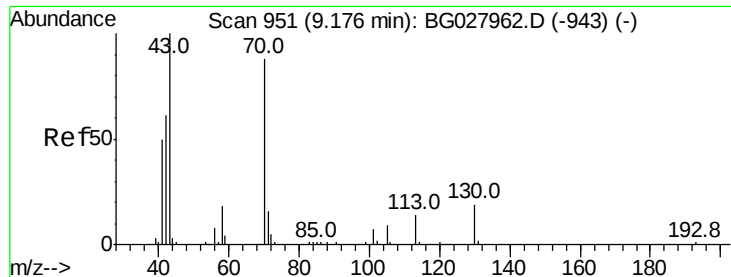

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.242 ng/ul
 RT: 9.08 min Scan# 934
 Delta R.T. -0.10 min
 Lab File: BG027963.D
 Acq: 19 Jul 2017 15:37

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Tot Ion: 70 Resp: 2631
 Ion Ratio Lower Upper
 70 100
 42 424.1 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

