

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027980.D
 Acq On : 20 Jul 2017 2:51
 Operator : SJ/JU
 Sample : I4213-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B40

Quant Time: Jul 20 06:02:54 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	55911	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	220267	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.97	164	155136	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	427028	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	542156	20.00	ng/ul	0.00
83) Perylene-d12	25.58	264	511616	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.87	96	6204	6.12	ng/uL	0.00
5) Phenol-d5	7.52	99	126506	27.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	80609	30.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	110637	30.65	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	110293	29.00	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	53645	33.10	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	65858	33.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.81	165	119597	31.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	139644	40.49	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	474311	35.27	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	508211	33.24	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	52105	26.75	ng/ul	0.00
57) Fluorene-d10	15.96	176	426751	33.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	69819	23.54	ng/ul	0.00
70) Anthracene-d10	17.82	188	731848	35.54	ng/ul	0.00
76) Pyrene-d10	20.09	212	903604	37.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.34	264	874940	36.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.41	163	65595	5.356	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027980.D
Acq On : 20 Jul 2017 2:51
Operator : SJ/JU
Sample : I4213-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B40

Quant Time: Jul 20 06:02:54 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

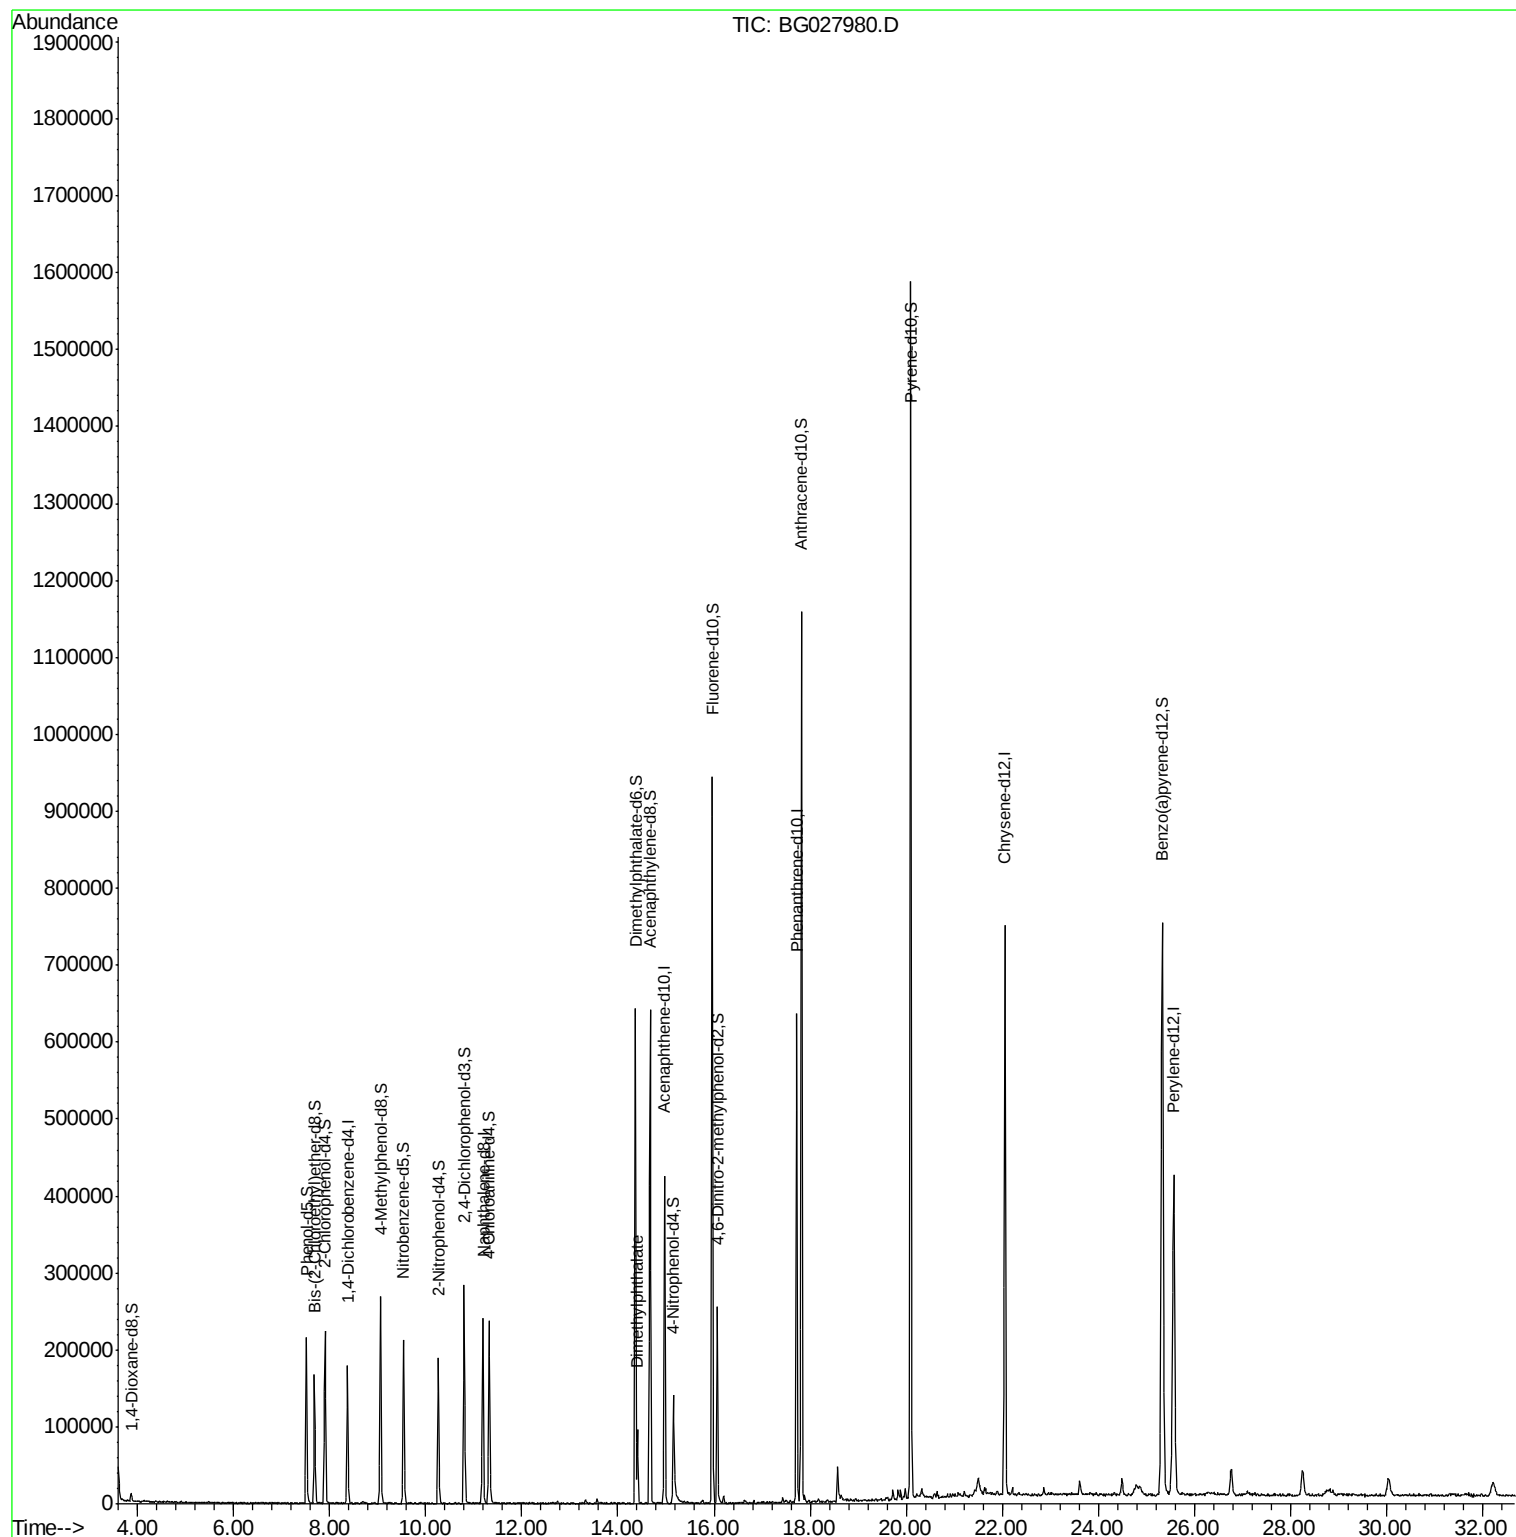

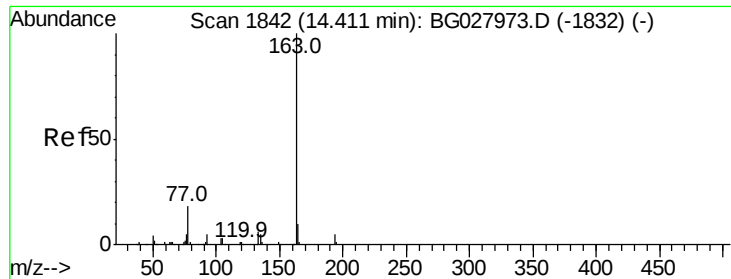

#44

Dimethylphthalate

Concen: 5.356 ng/ul

RT: 14.41 min Scan# 1841

Delta R.T. -0.00 min

Lab File: BG027980.D

Acq: 20 Jul 2017 2:51

Instrument :

BNA_G

ClientSampleId :

C0B40


Tot Ion:163 Resp: 65595

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 12.3 9.0 13.4

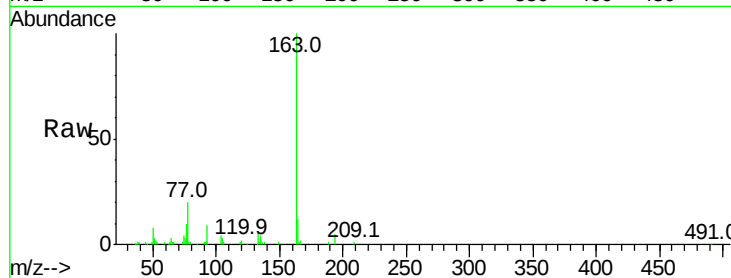

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

