

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027982.D
 Acq On : 20 Jul 2017 4:10
 Operator : SJ/JU
 Sample : I4213-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B72

Quant Time: Jul 20 06:03:17 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	52660	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	212322	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	148579	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	414631	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	535980	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	515461	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.86	96	4267	4.47	ng/uL	0.00
5) Phenol-d5	7.51	99	103706	23.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	72326	28.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	95949	28.22	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	95210	26.58	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	47384	30.33	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	57371	30.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	102773	27.95	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	125880	37.86	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	420345	32.63	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	439007	29.98	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	43851	23.51	ng/ul	0.00
57) Fluorene-d10	15.96	176	370485	30.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	63501	22.05	ng/ul	0.00
70) Anthracene-d10	17.82	188	656144	32.82	ng/ul	0.00
76) Pyrene-d10	20.09	212	848468	35.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	815622	33.88	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.41	163	54411	4.639	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027982.D
Acq On : 20 Jul 2017 4:10
Operator : SJ/JU
Sample : I4213-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B72

Quant Time: Jul 20 06:03:17 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

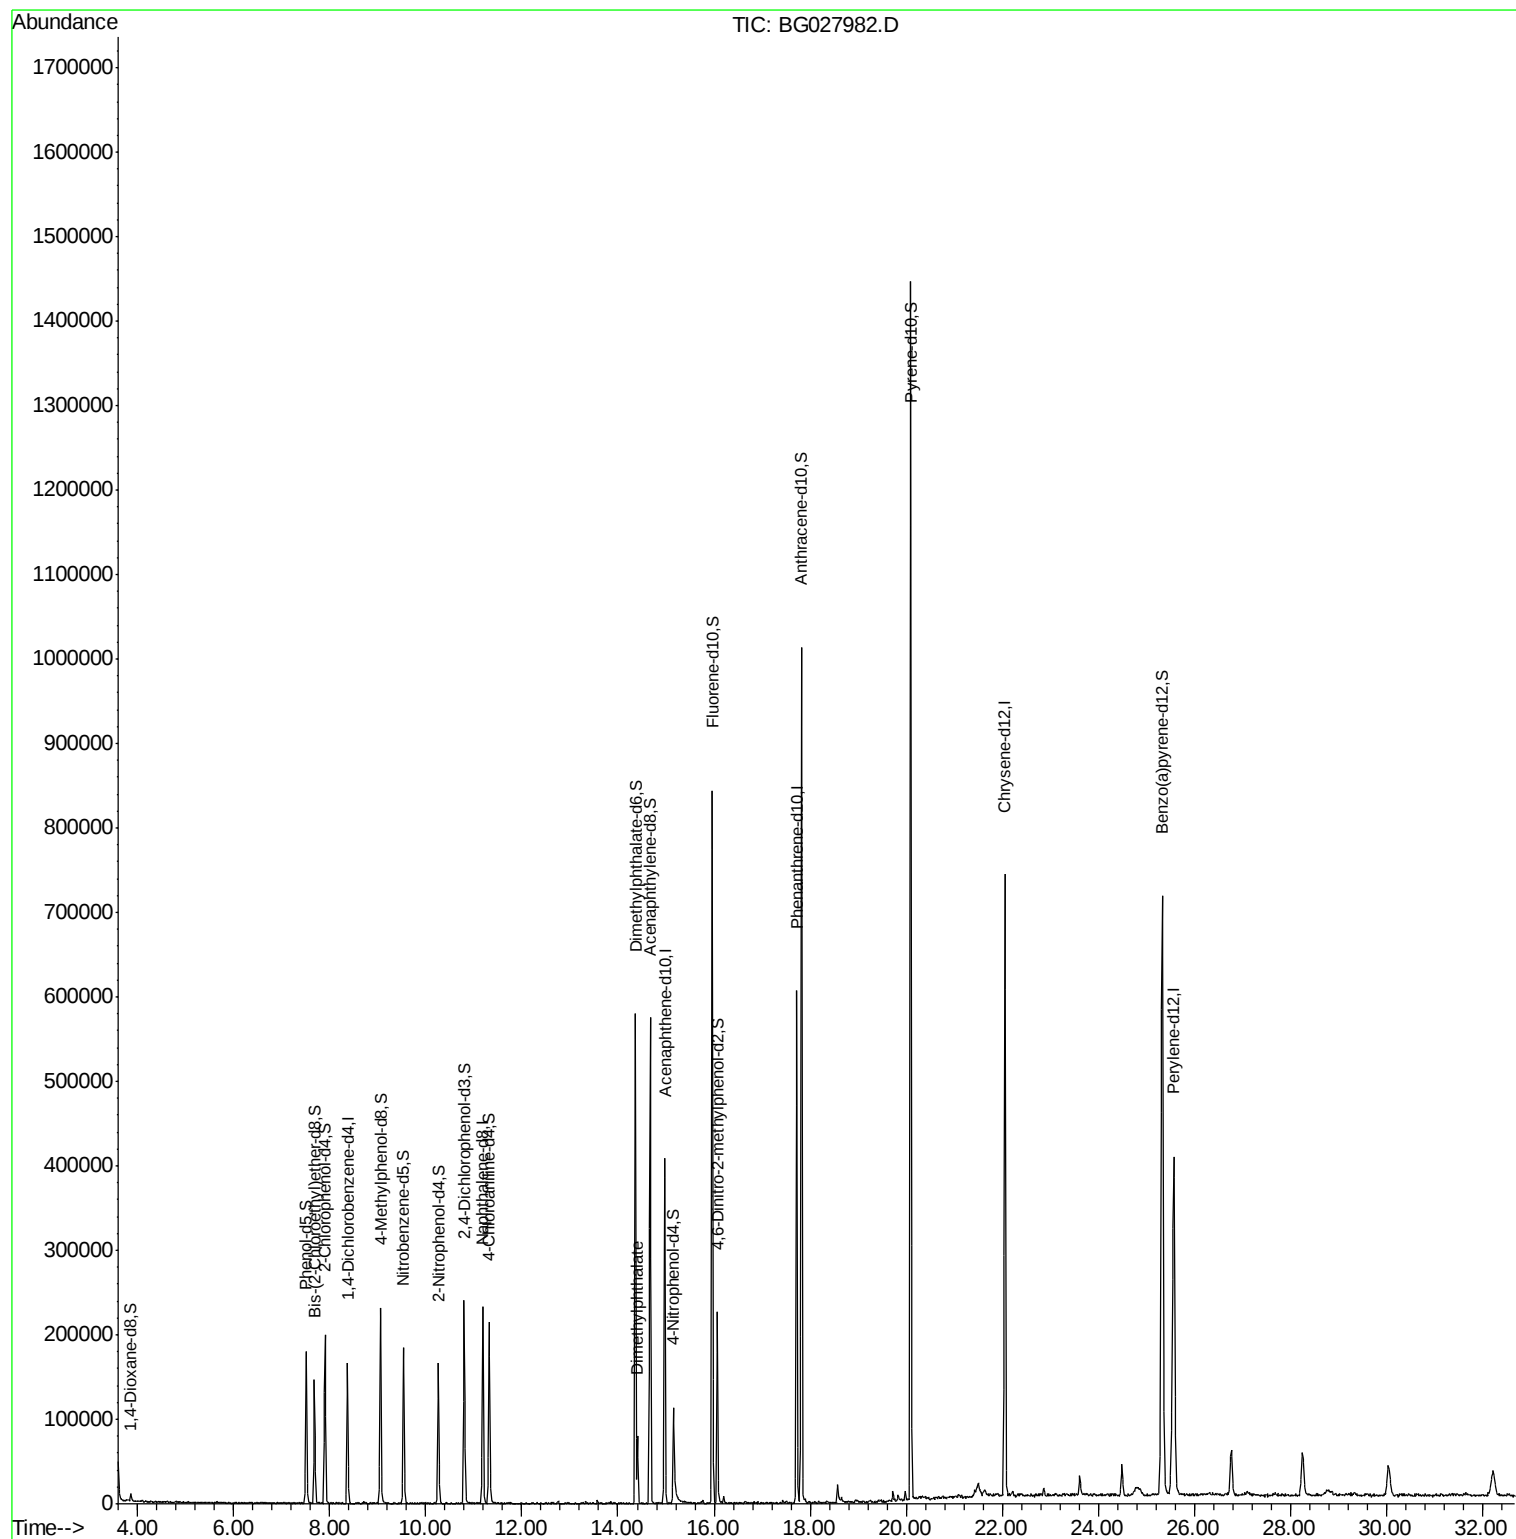

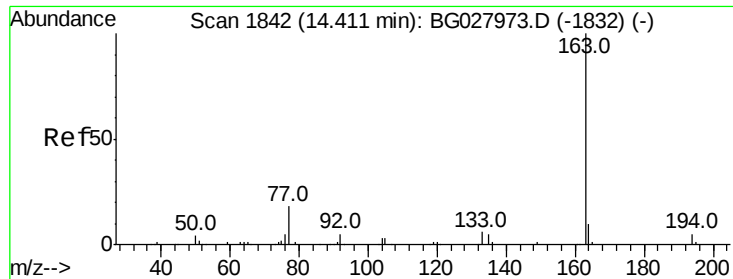

#44

Dimethylphthalate

Concen: 4.639 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BG027982.D

Acq: 20 Jul 2017 4:10

Instrument :

BNA_G

ClientSampleId :

C0B72


Tot Ion:163 Resp: 54411

Ion Ratio Lower Upper

163 100

194 5.3 3.4 5.0#

164 9.8 9.0 13.4

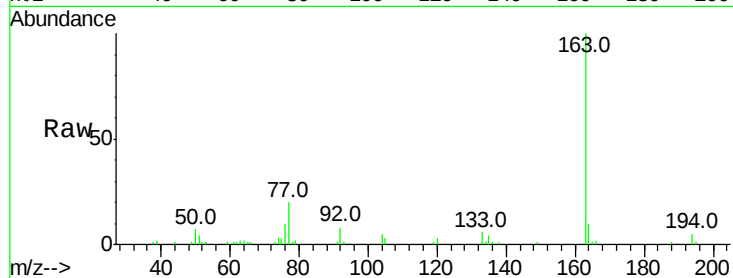

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

