

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027974.D
 Acq On : 19 Jul 2017 22:54
 Operator : SJ/JU
 Sample : I4213-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B34

Quant Time: Jul 20 06:01:38 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	61793	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	251081	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	172356	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	449098	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	579746	20.00	ng/ul	0.00
83) Perylene-d12	25.58	264	543008	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.87	96	5182	4.62	ng/uL	0.00
5) Phenol-d5	7.51	99	101202	19.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	64968	22.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	89083	22.33	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	89556	21.31	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	42901	23.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	51635	23.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	98047	22.54	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	113124	28.77	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	382158	25.58	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	408294	24.04	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	18453	8.53	ng/ul	0.00
57) Fluorene-d10	15.96	176	338455	24.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	28351	9.09	ng/ul	0.00
70) Anthracene-d10	17.82	188	547991	25.30	ng/ul	0.00
76) Pyrene-d10	20.09	212	682526	26.20	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	663103	26.15	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.41	163	59679	4.386	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027974.D
Acq On : 19 Jul 2017 22:54
Operator : SJ/JU
Sample : I4213-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B34

Quant Time: Jul 20 06:01:38 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

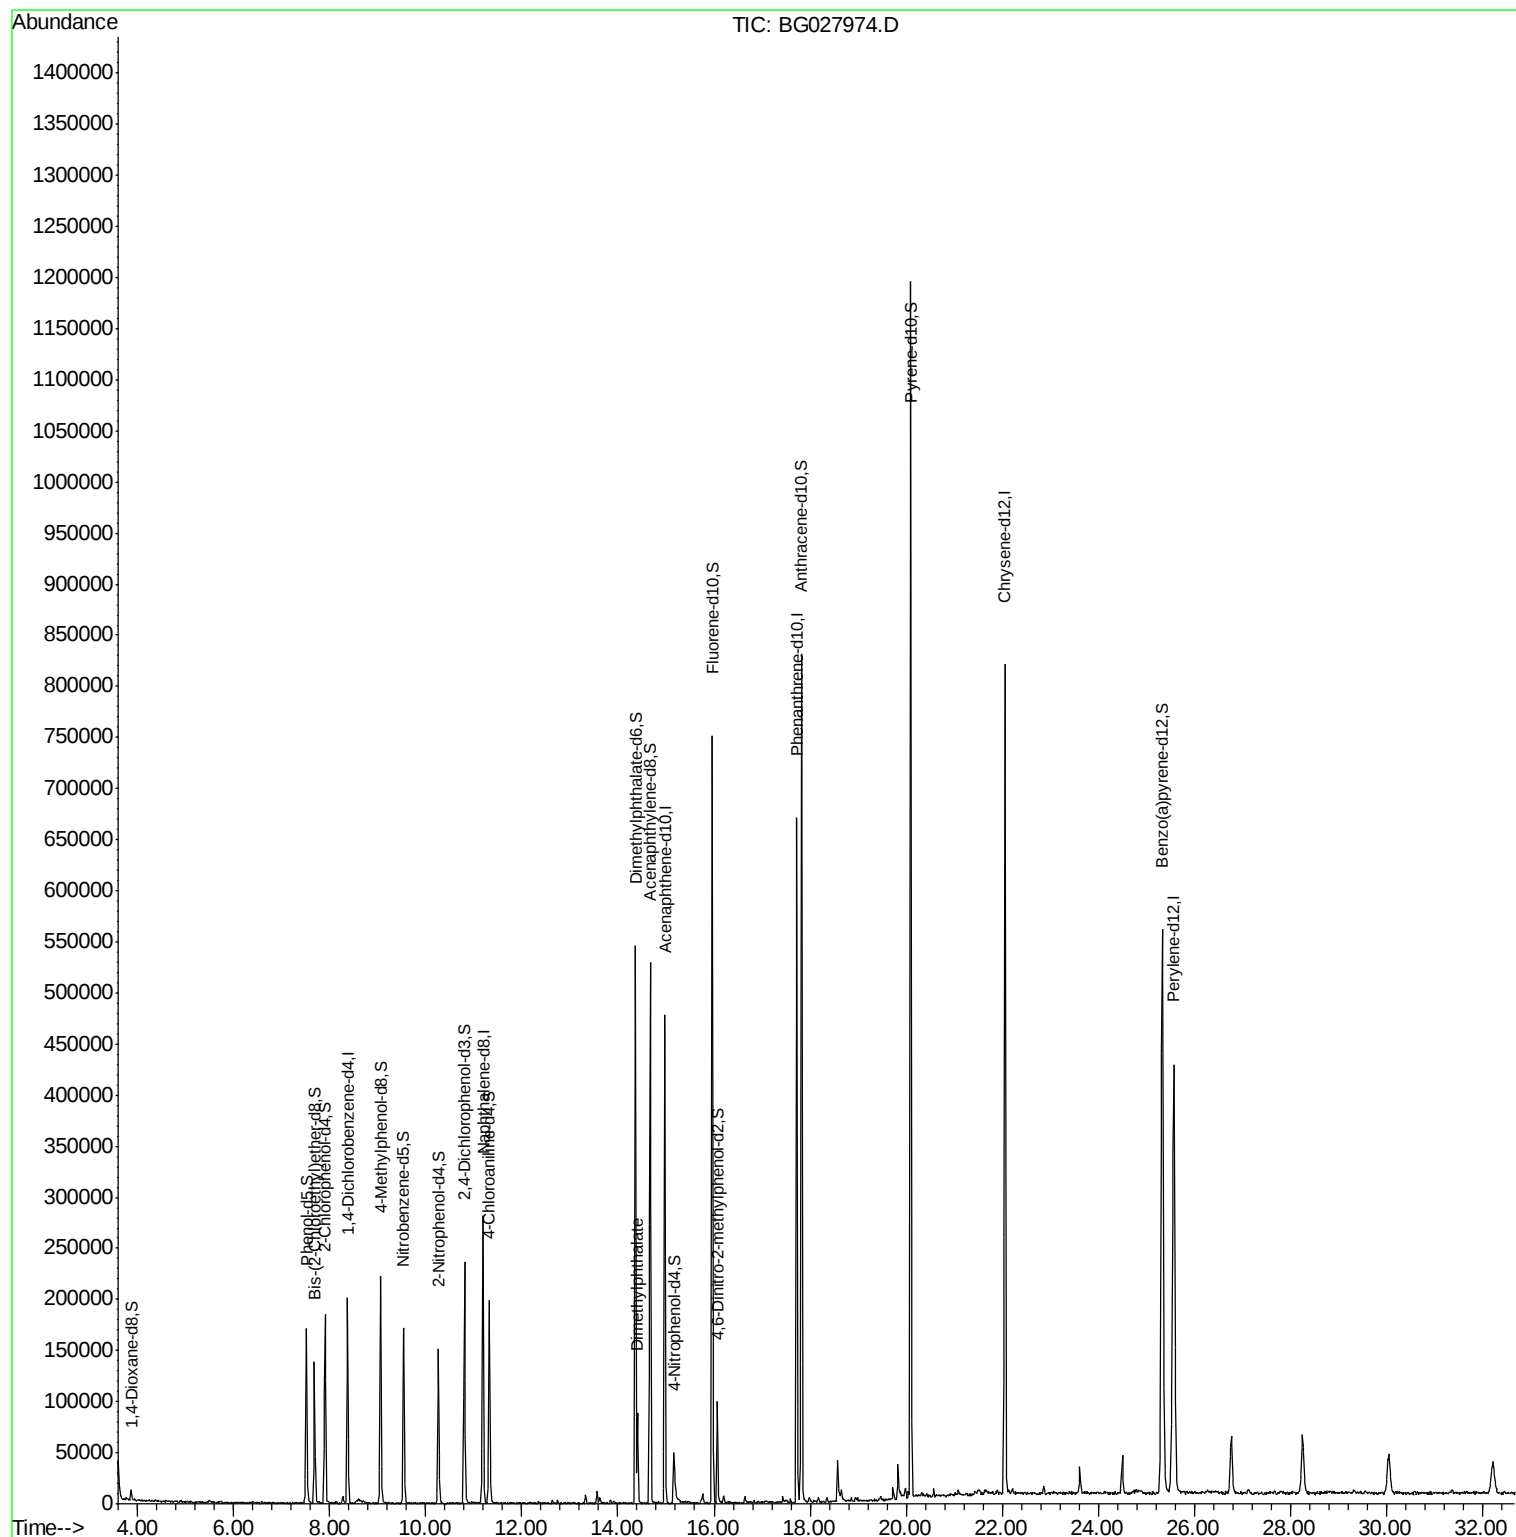

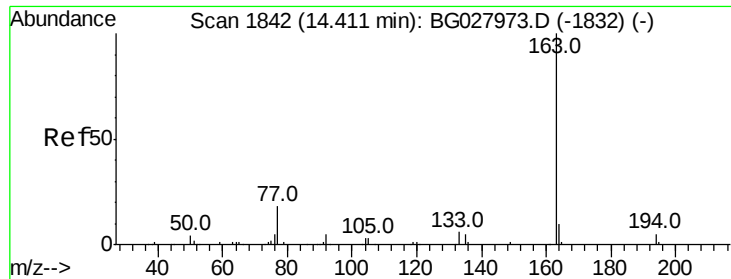

#44

Dimethylphthalate

Concen: 4.386 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BG027974.D

Acq: 19 Jul 2017 22:54

Instrument :

BNA_G

ClientSampleId :

C0B34


Tot Ion:163 Resp: 59679

Ion Ratio Lower Upper

163 100

194 5.5 3.4 5.0#

164 8.2 9.0 13.4#

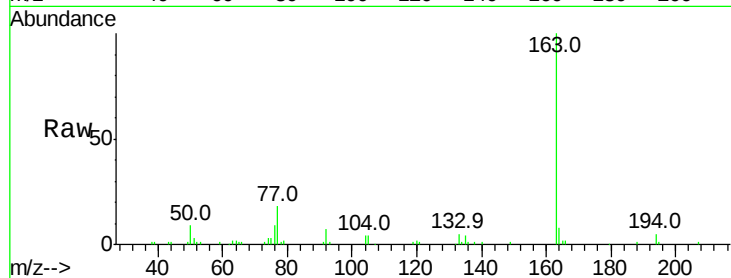

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

