

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027975.D
 Acq On : 19 Jul 2017 23:33
 Operator : SJ/JU
 Sample : I4213-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B35

Quant Time: Jul 20 06:09:20 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	68236	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	287157	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	200029	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	515055	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	633734	20.00	ng/ul	0.00
83) Perylene-d12	25.58	264	596100	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.86	96	6961	5.62	ng/uL	0.00
5) Phenol-d5	7.52	99	165609	29.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.69	67	102958	31.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	137041	31.11	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	144041	31.03	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	69417	32.85	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	84543	33.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.81	165	160970	32.36	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	174202	38.74	ng/ul	0.00
43) Dimethylphthalate-d6	14.37	166	612692	35.33	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	669928	33.99	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	66964	26.67	ng/ul	0.00
57) Fluorene-d10	15.96	176	551301	33.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	90216	25.22	ng/ul	0.00
70) Anthracene-d10	17.82	188	888067	35.75	ng/ul	0.00
76) Pyrene-d10	20.09	212	1078420	37.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	1042006	37.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.41	163	71650	4.537	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027975.D
Acq On : 19 Jul 2017 23:33
Operator : SJ/JU
Sample : I4213-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jul 20 06:09:20 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

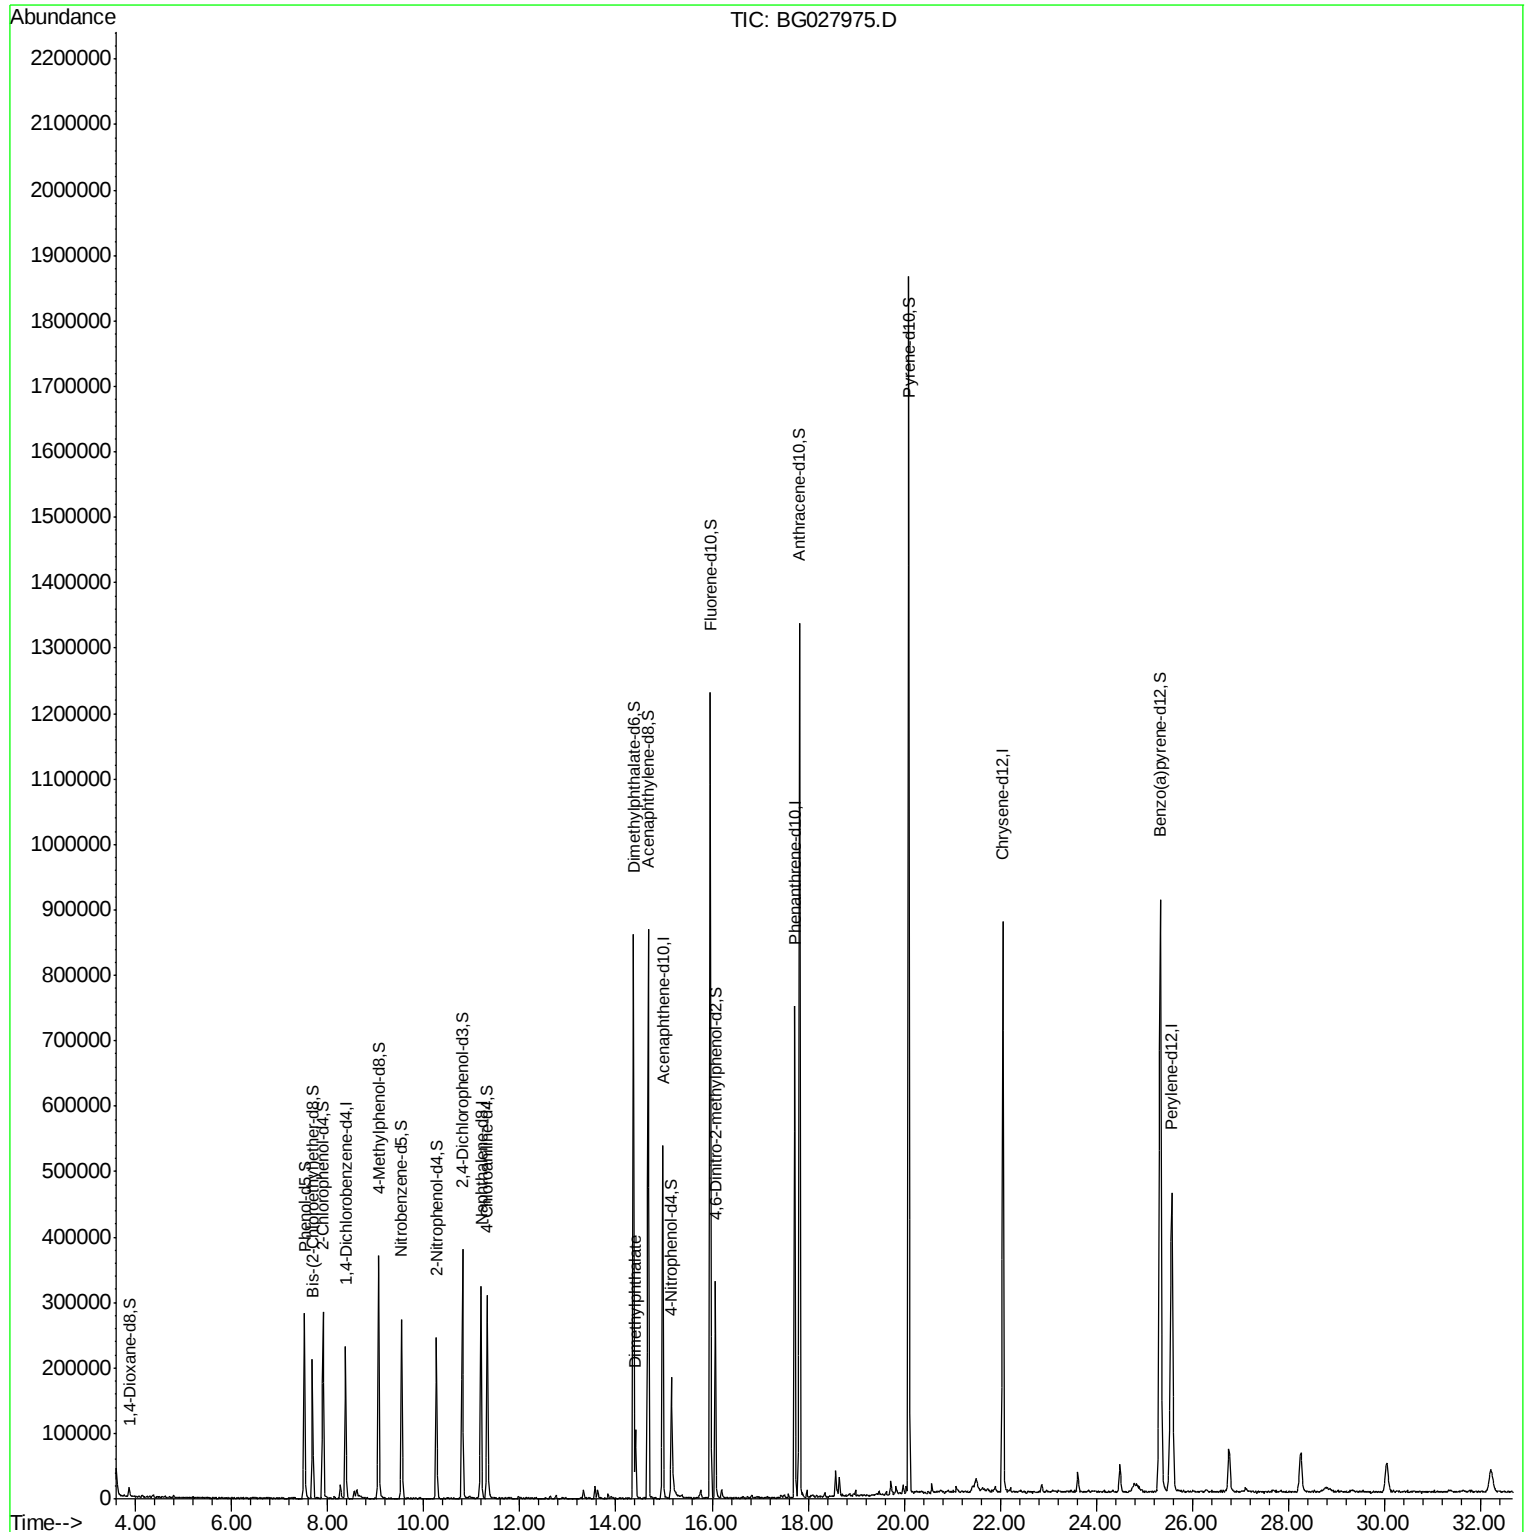

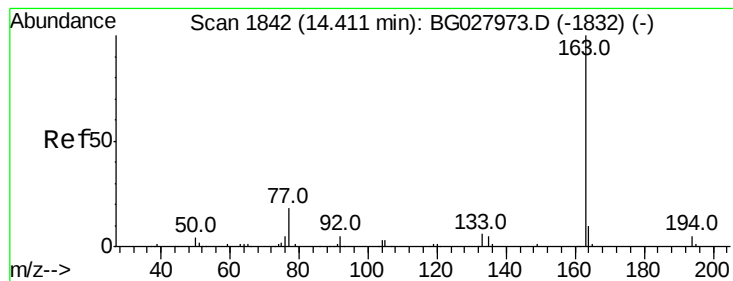

#44

Dimethylphthalate

Concen: 4.537 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BG027975.D

Acq: 19 Jul 2017 23:33

Instrument :

BNA_G

ClientSampleId :

C0B35


Tot Ion:163 Resp: 71650

Ion Ratio Lower Upper

163 100

194 5.5 3.4 5.0#

164 11.0 9.0 13.4

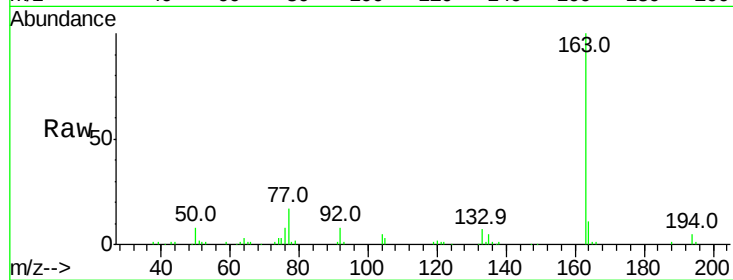

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

