

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027978.D
 Acq On : 20 Jul 2017 1:32
 Operator : SJ/JU
 Sample : I4213-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B38

Quant Time: Jul 20 06:02:30 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	58783	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	230719	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	149886	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.72	188	408550	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	536785	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	514084	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.86	96	2398	2.25	ng/uL	-0.01
5) Phenol-d5	7.51	99	47467	9.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	29188	10.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	40579	10.69	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	37281	9.32	ng/ul	0.00
19) Nitrobenzene-d5	9.54	128	18293	10.78	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	18107	8.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	41304	10.34	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	49076	13.58	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	162821	12.53	ng/ul	0.00
46) Acenaphthylene-d8	14.67	160	173625	11.76	ng/ul	0.00
51) 4-Nitrophenol-d4	15.17	143	4449	2.36	ng/ul	0.02
57) Fluorene-d10	15.96	176	149368	12.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	3797	1.34	ng/ul	0.00
70) Anthracene-d10	17.82	188	254055	12.89	ng/ul	0.00
76) Pyrene-d10	20.09	212	329669	13.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	314292	13.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.41	163	31118	2.630	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027978.D
Acq On : 20 Jul 2017 1:32
Operator : SJ/JU
Sample : I4213-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B38

Quant Time: Jul 20 06:02:30 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

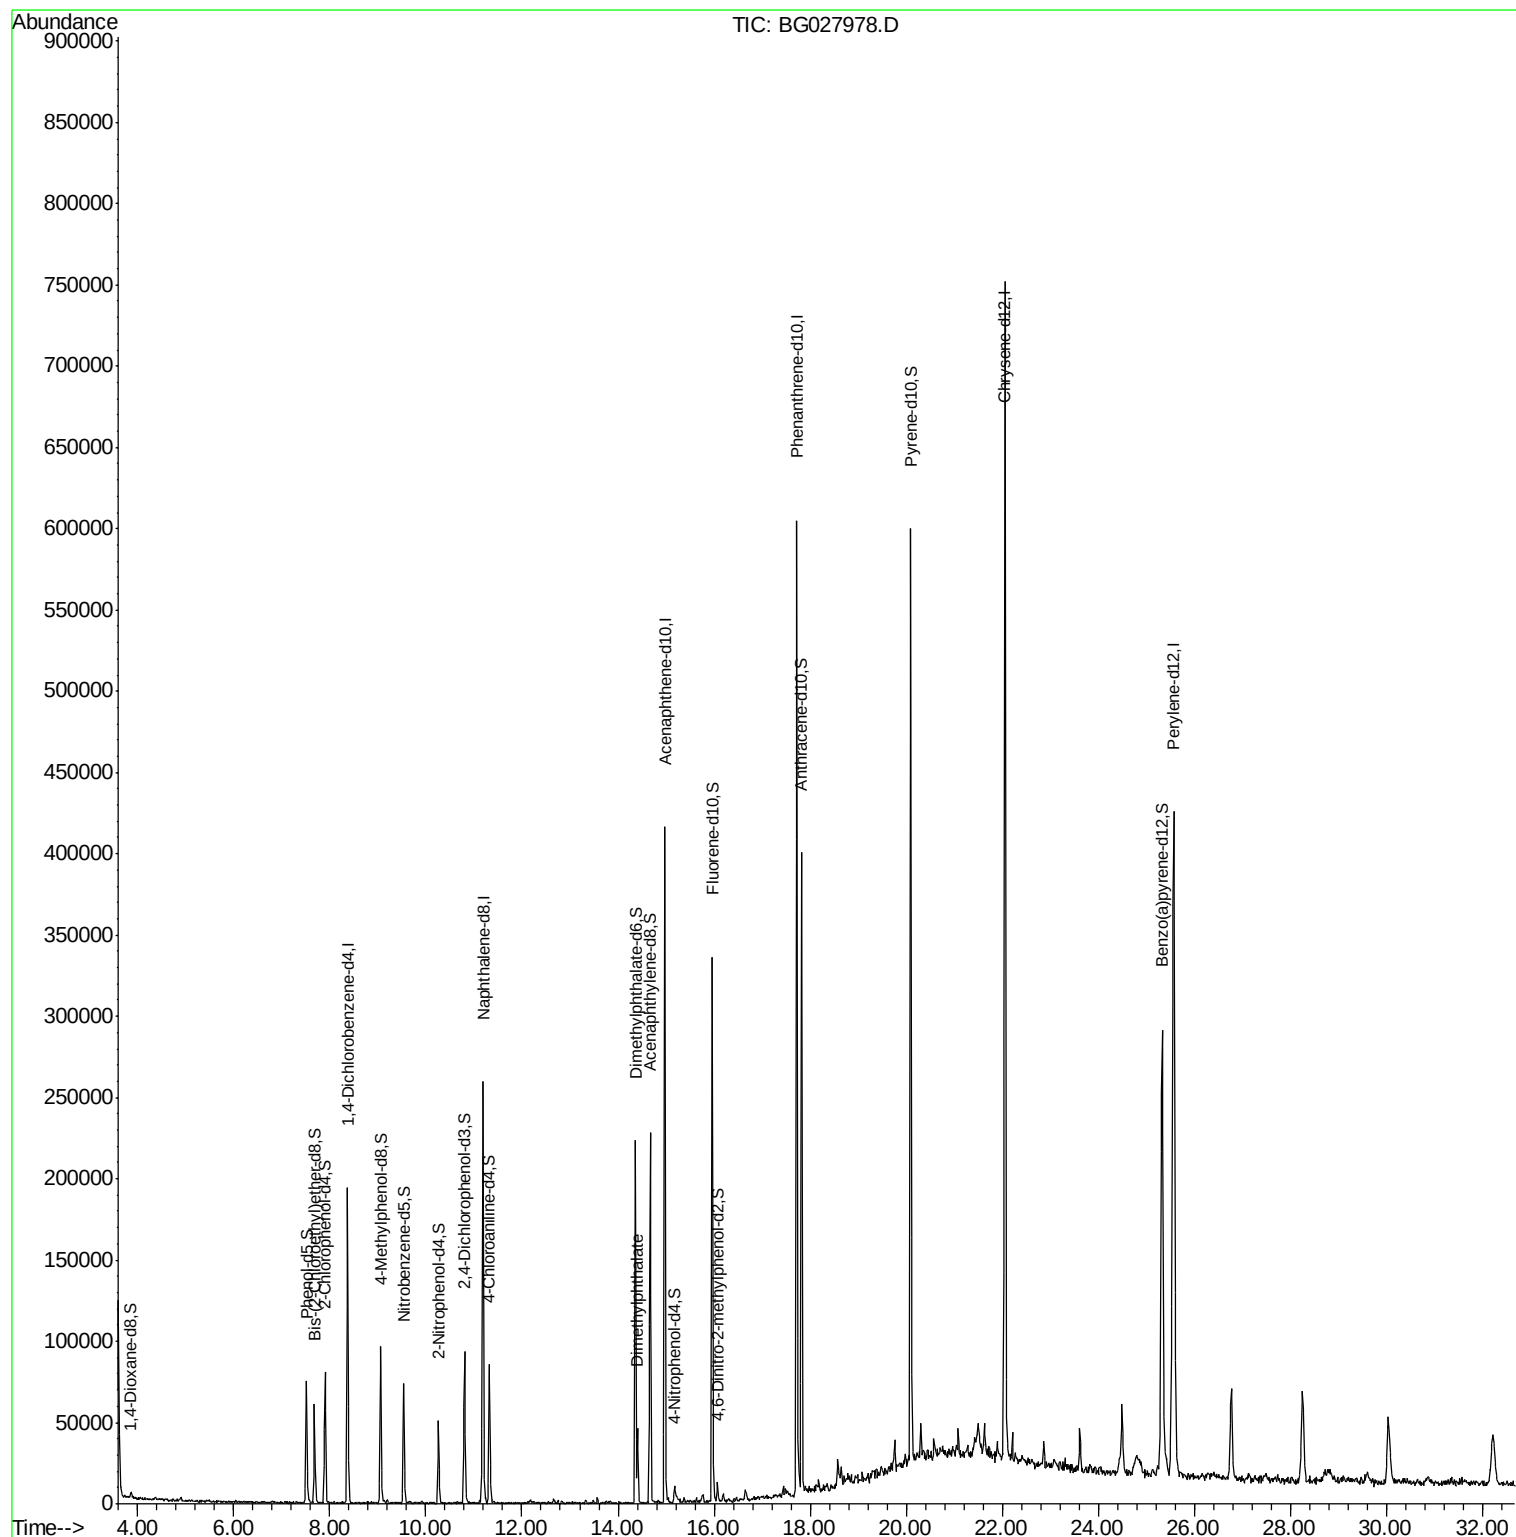

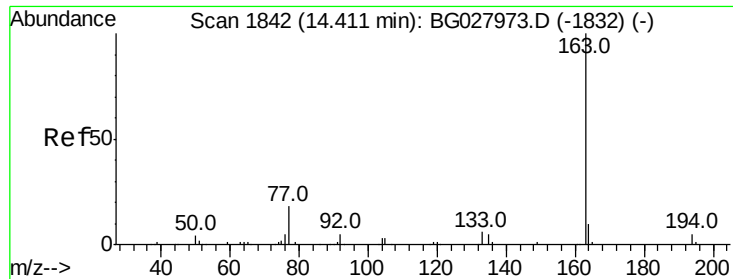

#44

Dimethylphthalate

Concen: 2.630 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BG027978.D

Acq: 20 Jul 2017 1:32

Instrument :

BNA_G

ClientSampleId :

C0B38


Tot Ion:163 Resp: 31118

Ion Ratio Lower Upper

163 100

194 5.8 3.4 5.0#

164 9.0 9.0 13.4

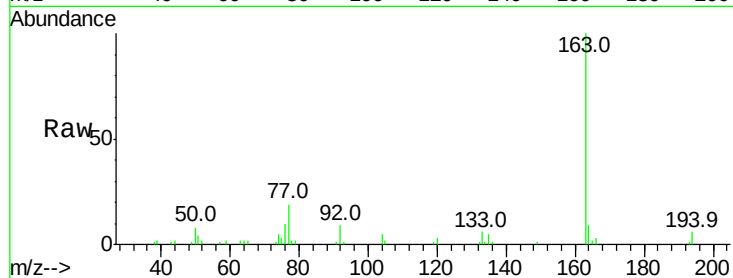

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

