

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
 Data File : BG027986.D
 Acq On : 20 Jul 2017 6:48
 Operator : SJ/JU
 Sample : I4214-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B75

Quant Time: Jul 20 07:24:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 20 05:55:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	52570	20.00	ng/ul	0.00
18) Naphthalene-d8	11.19	136	215733	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.98	164	151073	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.73	188	402820	20.00	ng/ul	0.00
75) Chrysene-d12	22.06	240	529638	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	507168	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.86	96	4693	4.92	ng/uL	-0.01
5) Phenol-d5	7.51	99	104530	24.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.68	67	68873	27.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.90	132	93122	27.44	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	91645	25.63	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	46000	28.98	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	57789	30.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	101144	27.07	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	122671	36.32	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	409540	31.27	ng/ul	0.00
46) Acenaphthylene-d8	14.68	160	437676	29.40	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	45201	23.83	ng/ul	0.00
57) Fluorene-d10	15.96	176	361058	29.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	64171	22.94	ng/ul	0.00
70) Anthracene-d10	17.82	188	617207	31.77	ng/ul	0.00
76) Pyrene-d10	20.10	212	793518	33.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.33	264	769500	32.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.41	163	71102	5.962	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG071917\
Data File : BG027986.D
Acq On : 20 Jul 2017 6:48
Operator : SJ/JU
Sample : I4214-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B75

Quant Time: Jul 20 07:24:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG071717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 20 05:55:18 2017
Response via : Initial Calibration

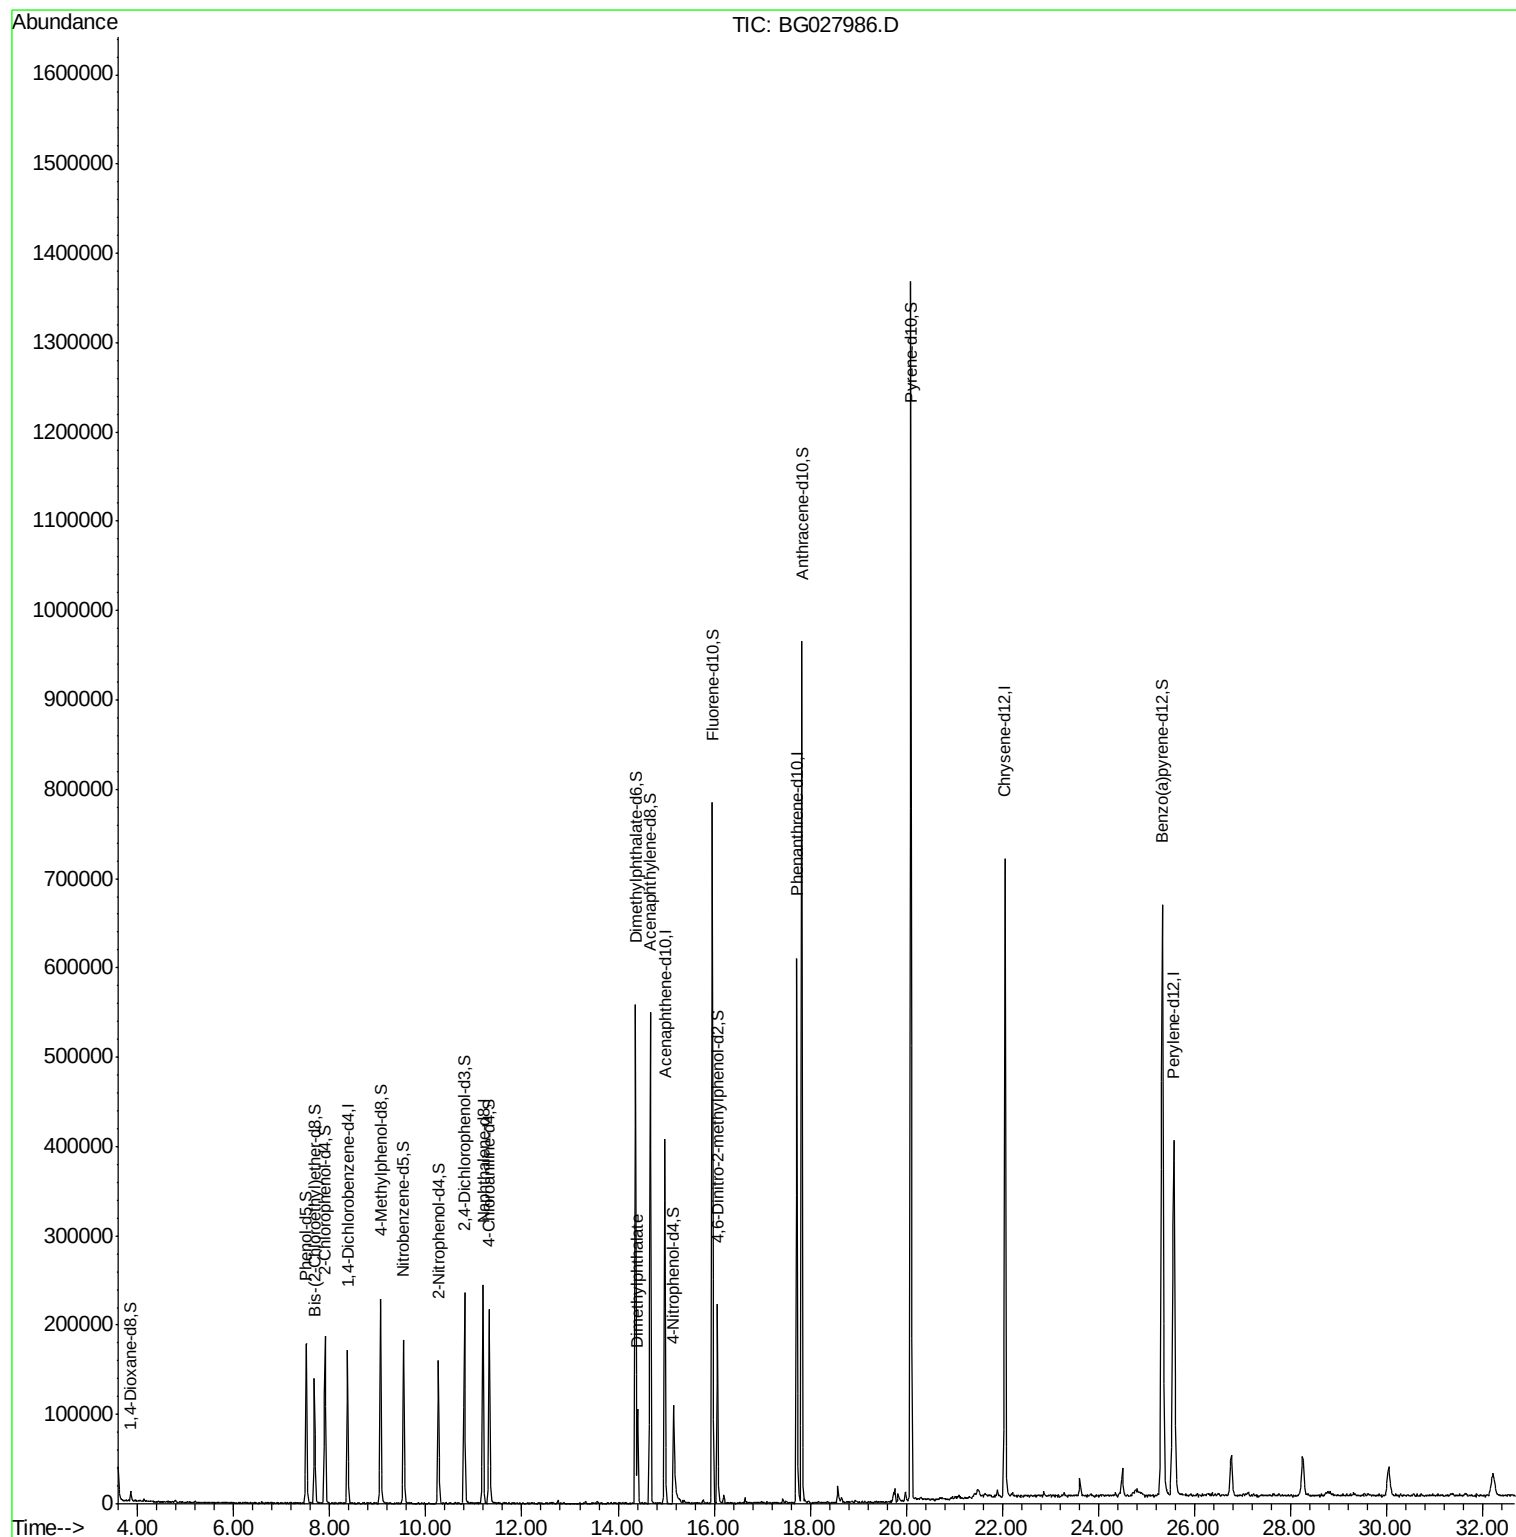

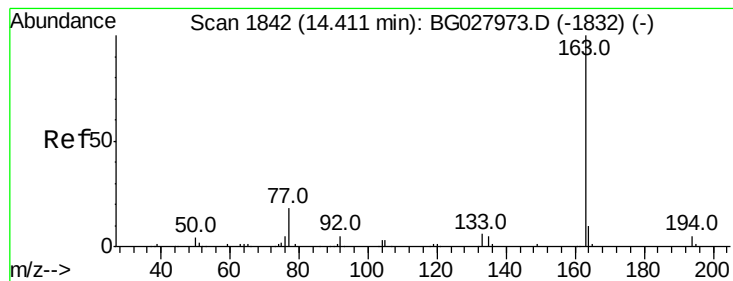

#44

Dimethylphthalate

Concen: 5.962 ng/ul

RT: 14.41 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BG027986.D

Acq: 20 Jul 2017 6:48

Instrument :

BNA_G

ClientSampleId :

C0B75


Tot Ion:163 Resp: 71102

Ion Ratio Lower Upper

163 100

194 6.0 3.4 5.0#

164 11.0 9.0 13.4

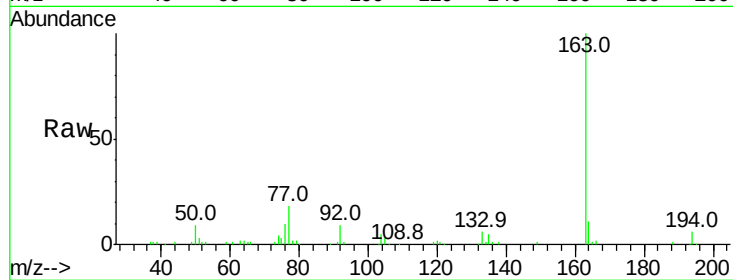

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

