

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071922\  
 Data File : BG054316.D  
 Acq On : 19 Jul 2022 10:05  
 Operator : CG/JU  
 Sample : PB145953BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB145953BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054316.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.568       | 364           | 371         | 383          | rBV      | 256302         | 431820        | 21.40%          | 6.815%        |
| 2         | 7.166       | 636           | 643         | 656          | rBV      | 263766         | 461675        | 22.88%          | 7.286%        |
| 3         | 8.000       | 778           | 785         | 792          | rBB      | 49533          | 86487         | 4.29%           | 1.365%        |
| 4         | 9.158       | 974           | 982         | 995          | rBB      | 156550         | 290833        | 14.41%          | 4.590%        |
| 5         | 10.809      | 1255          | 1263        | 1272         | rBV      | 62462          | 114390        | 5.67%           | 1.805%        |
| 6         | 13.253      | 1672          | 1679        | 1687         | rBV      | 505199         | 839064        | 41.58%          | 13.241%       |
| 7         | 14.634      | 1907          | 1914        | 1922         | rBB      | 116795         | 185597        | 9.20%           | 2.929%        |
| 8         | 16.120      | 2160          | 2167        | 2178         | rBV      | 493001         | 769876        | 38.15%          | 12.149%       |
| 9         | 17.377      | 2373          | 2381        | 2388         | rBV      | 183169         | 278953        | 13.82%          | 4.402%        |
| 10        | 19.986      | 2819          | 2825        | 2831         | rBV      | 1521869        | 2018123       | 100.00%         | 31.848%       |
| 11        | 21.637      | 3100          | 3106        | 3116         | rBV2     | 257524         | 425097        | 21.06%          | 6.709%        |
| 12        | 24.839      | 3640          | 3651        | 3664         | rBV      | 149202         | 434776        | 21.54%          | 6.861%        |




Sum of corrected areas: 6336691

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071922\  
Data File : BG054316.D  
Acq On : 19 Jul 2022 10:05  
Operator : CG/JU  
Sample : PB145953BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

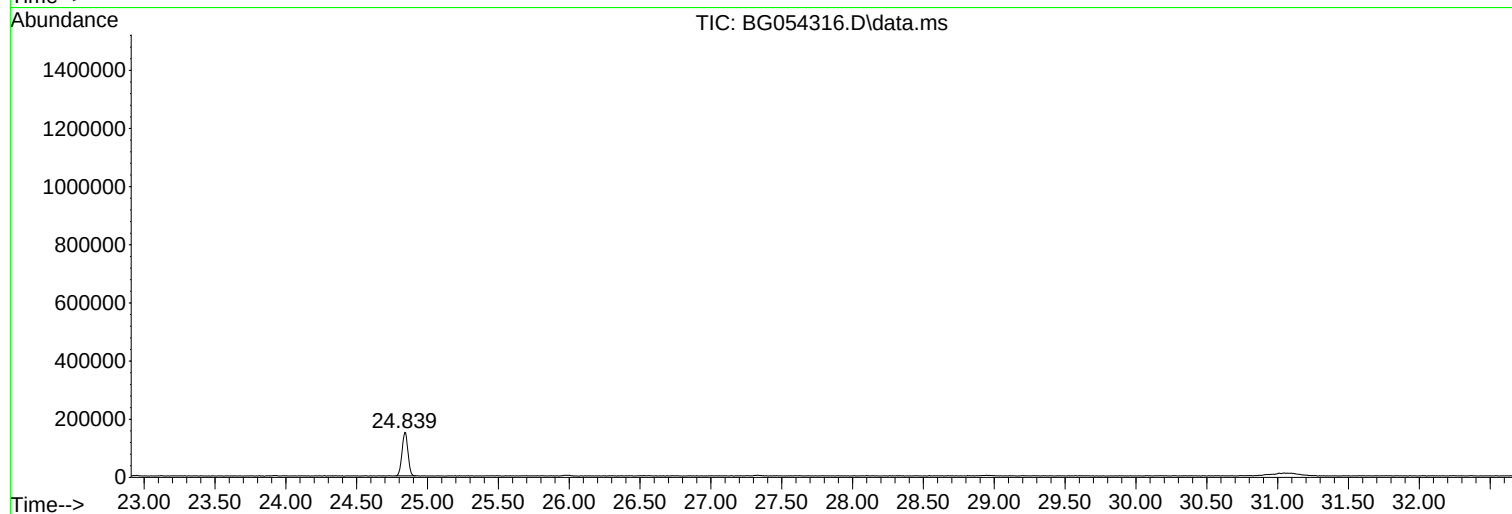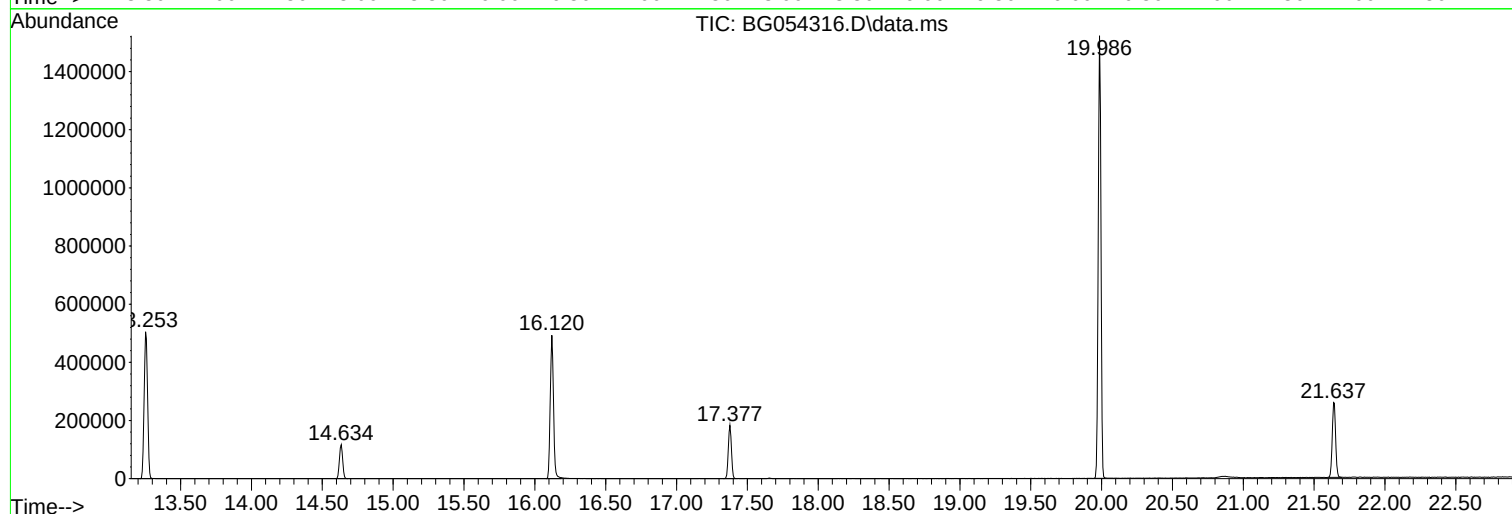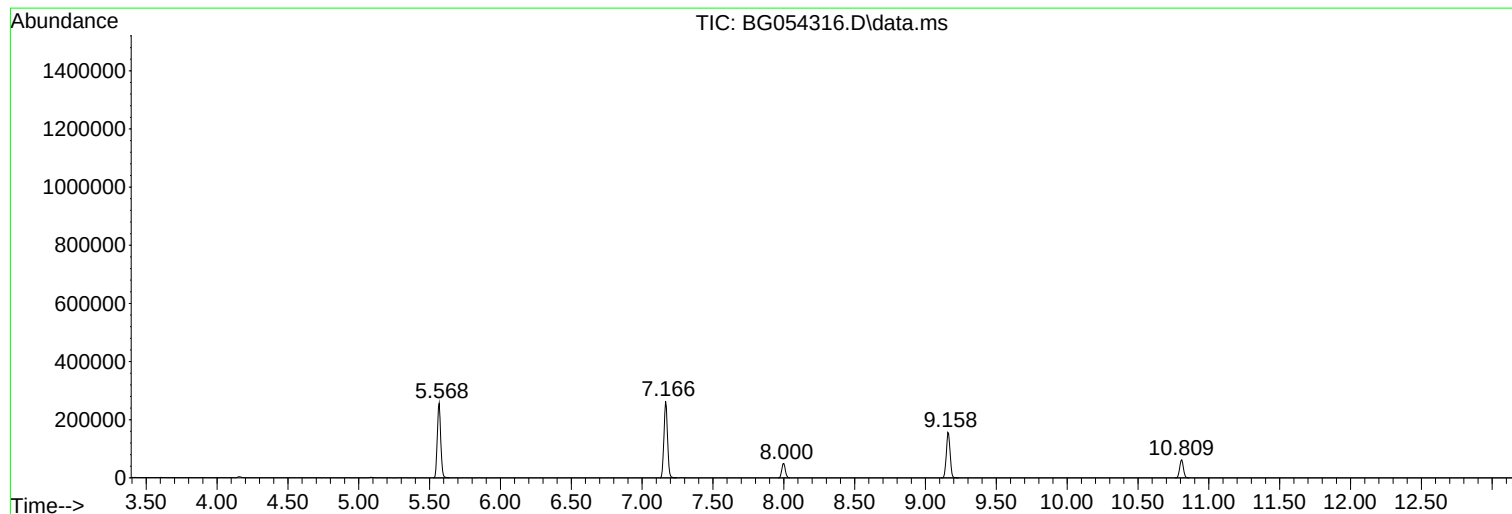

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071922\  
Data File : BG054316.D  
Acq On : 19 Jul 2022 10:05  
Operator : CG/JU  
Sample : PB145953BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG071922\  
Data File : BG054316.D  
Acq On : 19 Jul 2022 10:05  
Operator : CG/JU  
Sample : PB145953BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB145953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG071522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|