
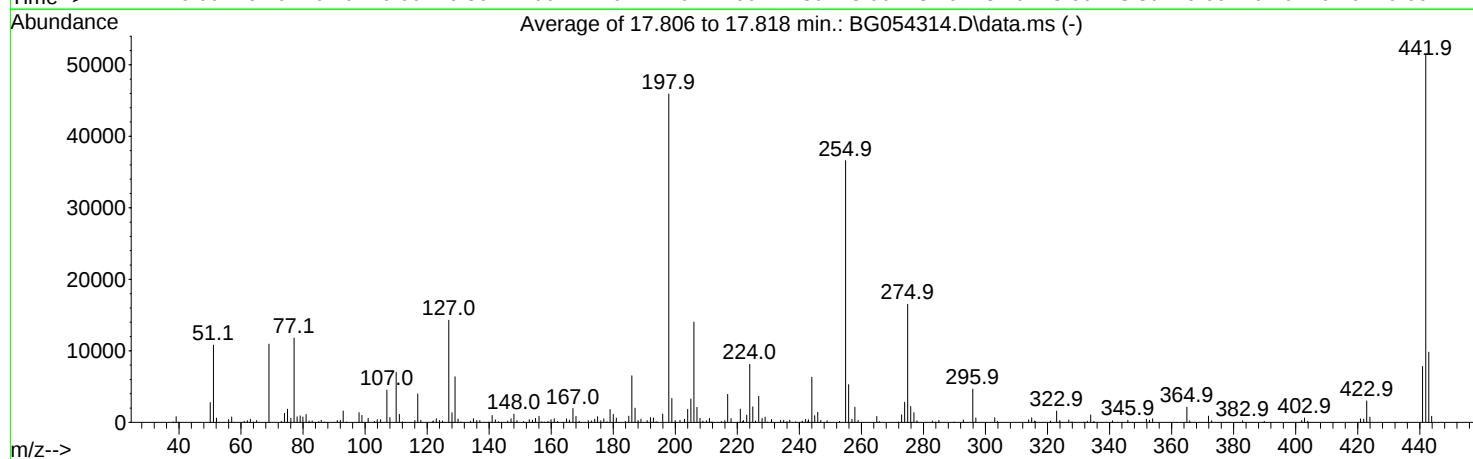


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071922\
 Data File : BG054314.D
 Acq On : 19 Jul 2022 8:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

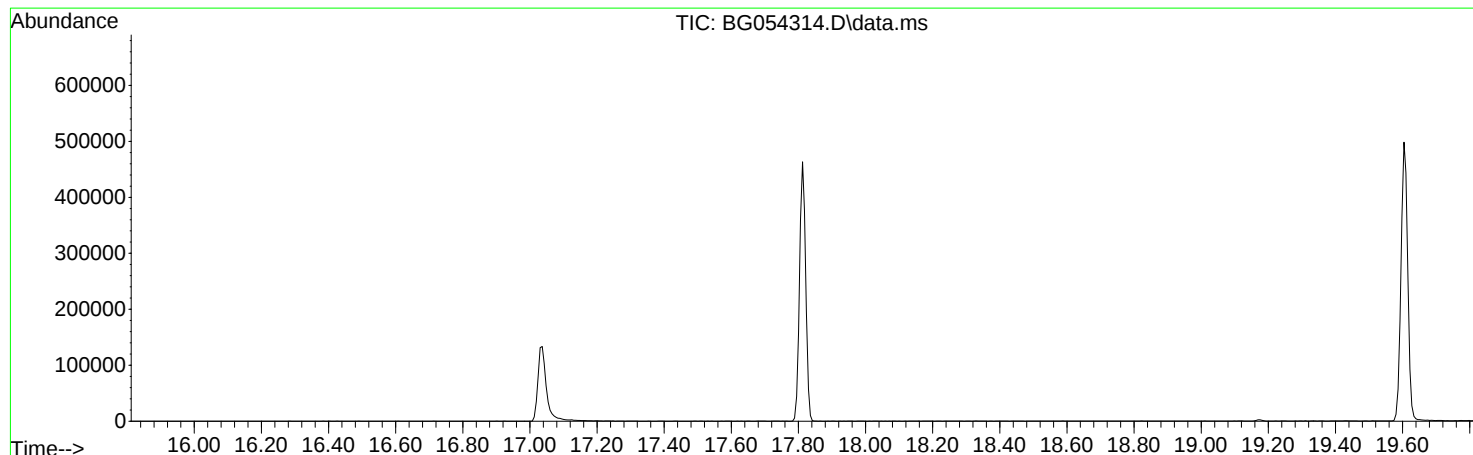




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.5	10805	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.8	10943	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.1	14285	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45915	PASS
199	198	5	9	7.3	3332	PASS
275	198	10	60	36.0	16522	PASS
365	198	1	100	4.6	2119	PASS
441	198	0.01	100	17.0	7800	PASS
442	442	50	100	100.0	51440	PASS
443	442	15	24	19.1	9834	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071922\
Data File : BG054314.D
Acq On : 19 Jul 2022 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 19 17:48:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

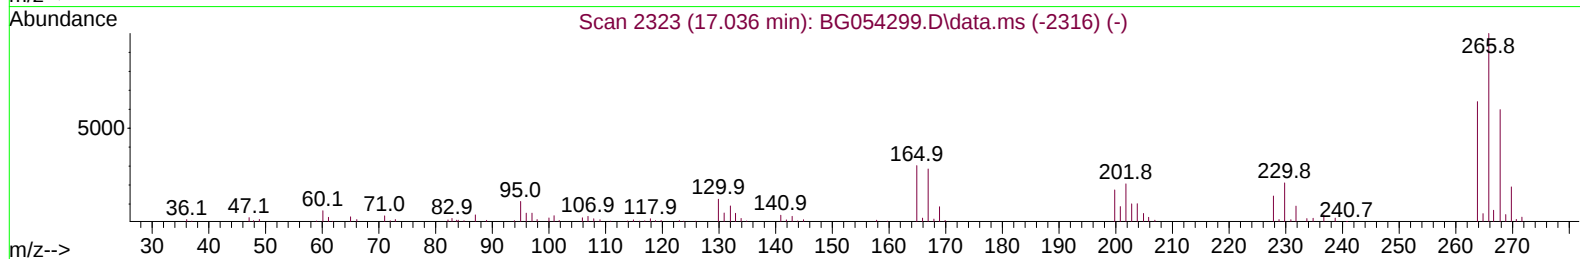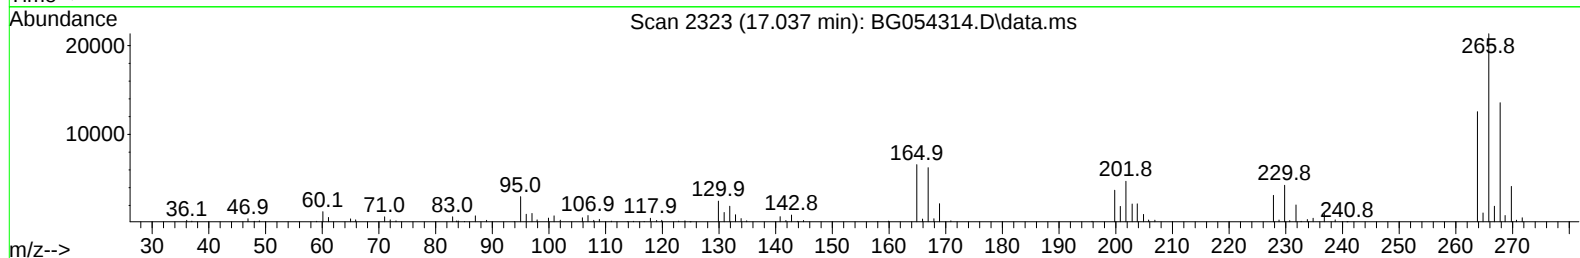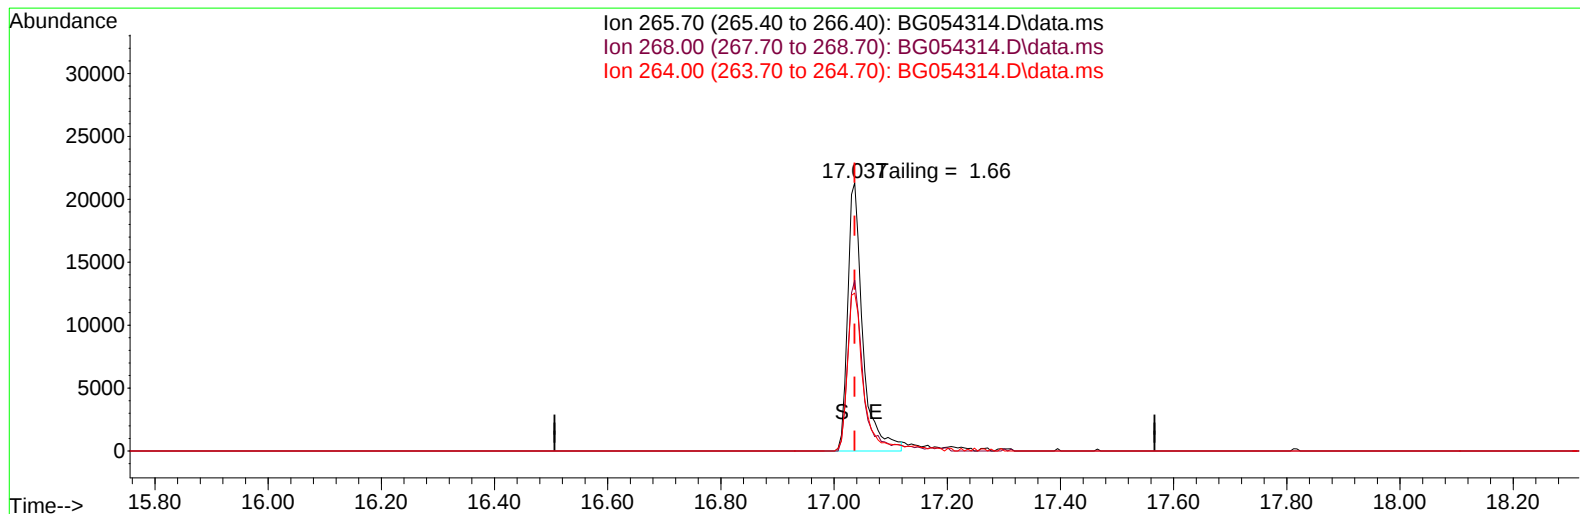

TIC: BG054314.D\data.ms

(70) Pentachlorophenol (C)

17.037min (+ 0.001) 20314.81 ng




response 41138

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.66
264.00	66.20	58.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071922\
Data File : BG054314.D
Acq On : 19 Jul 2022 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 19 17:48:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

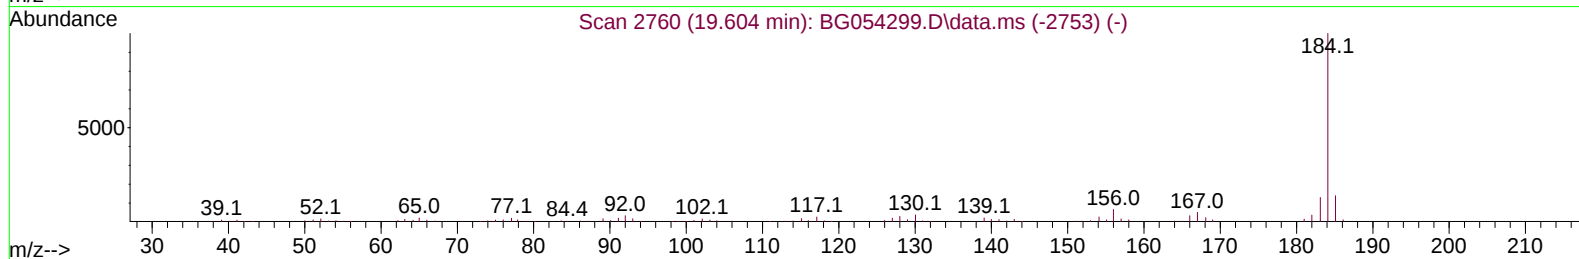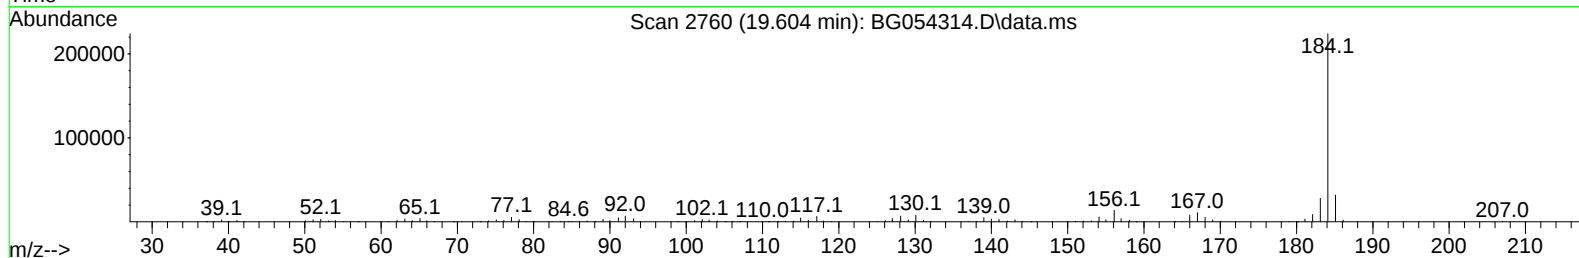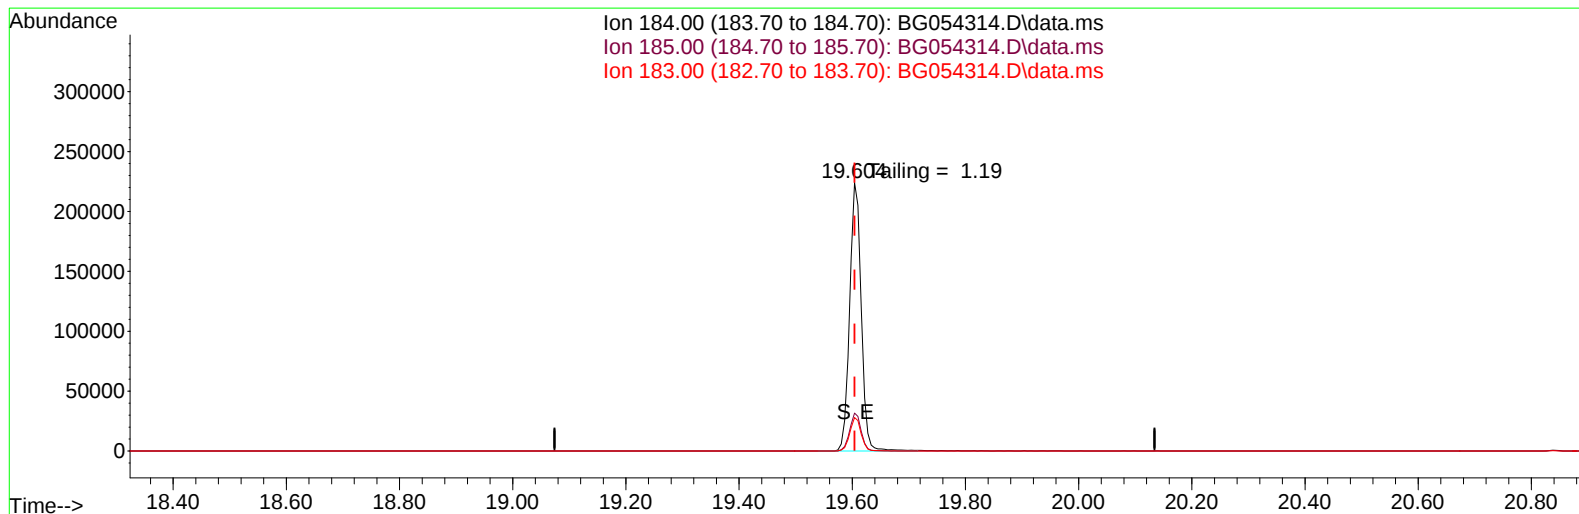

TIC: BG054314.D\data.ms

(77) Benzidine

19.604min (+ 0.000) 0.00 ng

response 318042

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.16
183.00	11.10	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/19/2022	BNA_G	<u>BG054314.D</u>
Compound Name	Response	Retention Time
DDT	198097	20.83
DDD	2460	20.4
DDE	141	19.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2601	200698	1.30

Instrument :
BNA_G
ClientSampleId :
DFTPP