




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

Quant Time: Jul 19 13:11:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

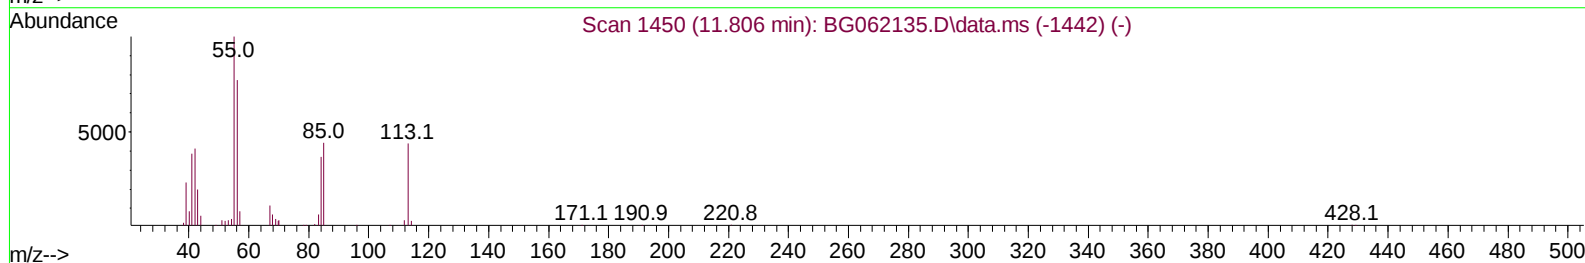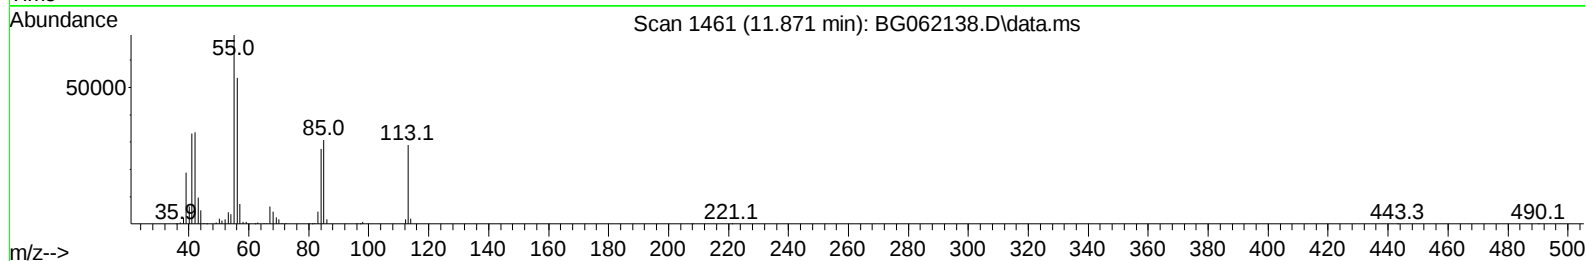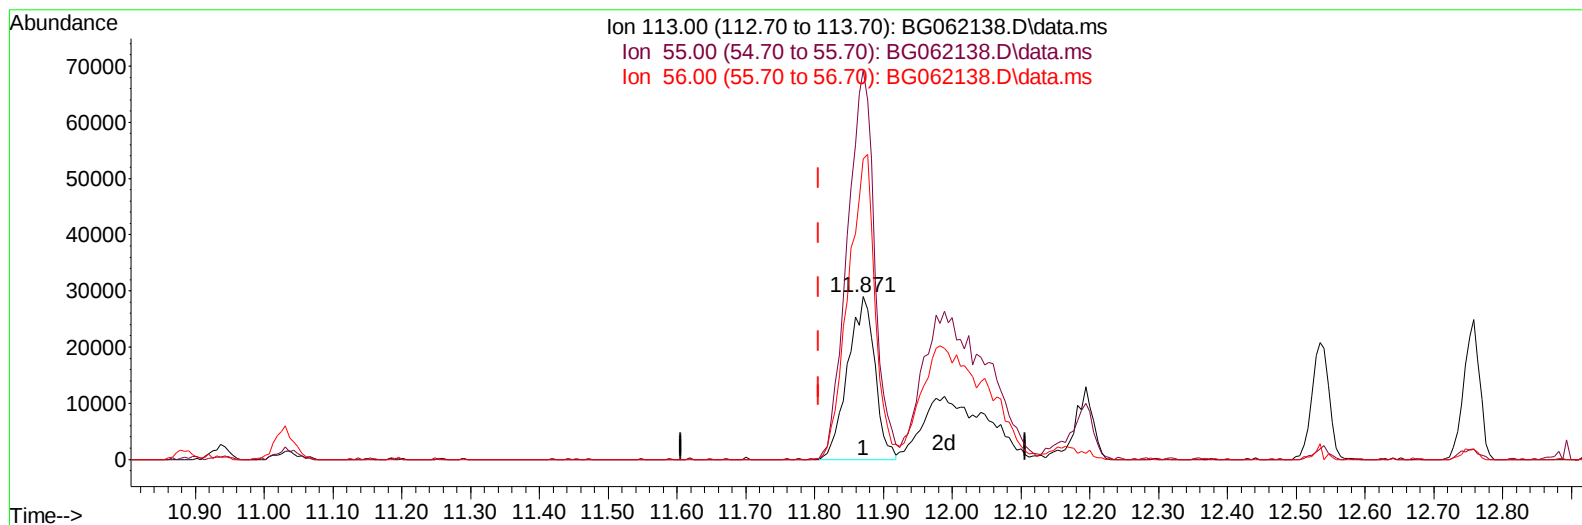

TIC: BG062138.D\data.ms

(34) Caprolactam

11.871min (+ 0.065) 74.06 ng/ul

response 79293

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	230.00	238.97
56.00	175.40	184.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Quant Time: Jul 19 13:11:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

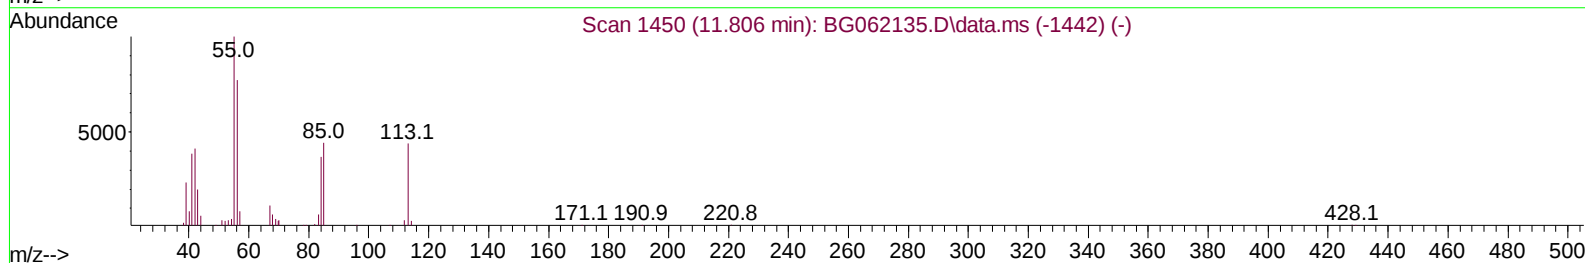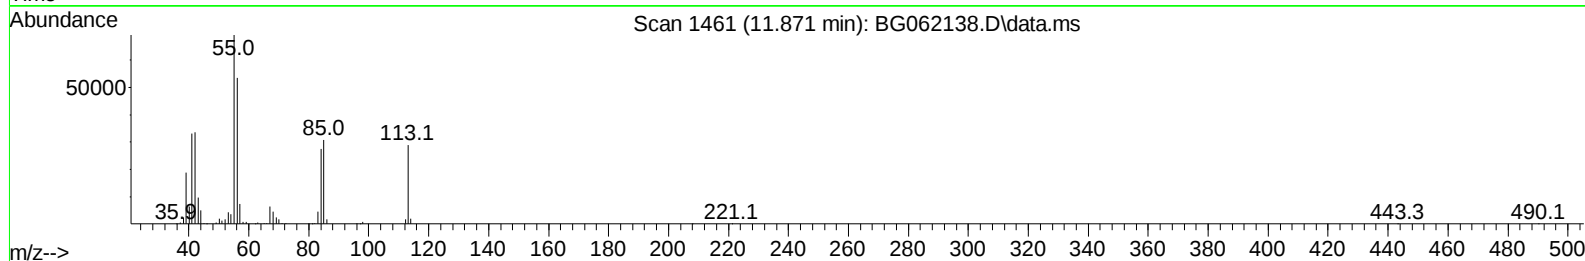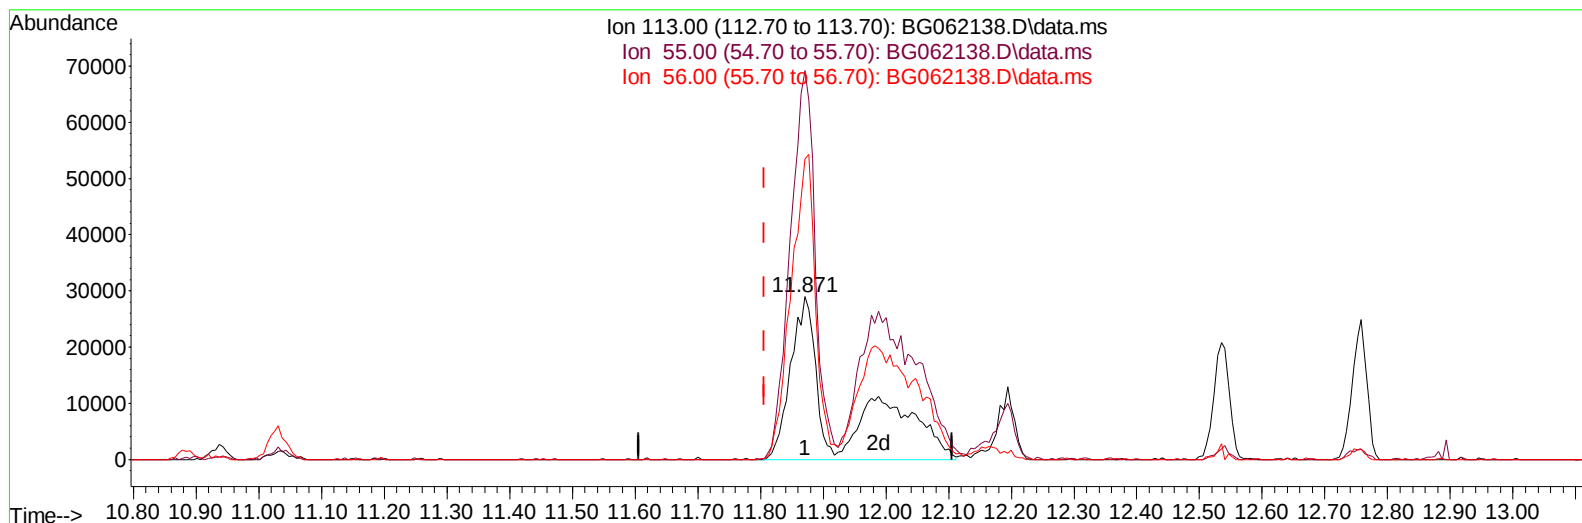

TIC: BG062138.D\data.ms

(34) Caprolactam

11.871min (+ 0.065) 141.12 ng/ul m

response 151099

Ion	Exp%	Act%
11		




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Quant Time: Jul 19 13:11:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

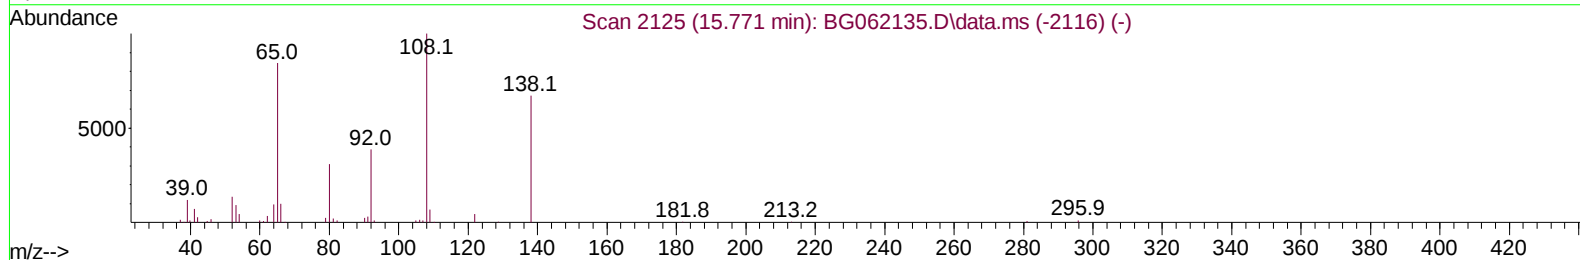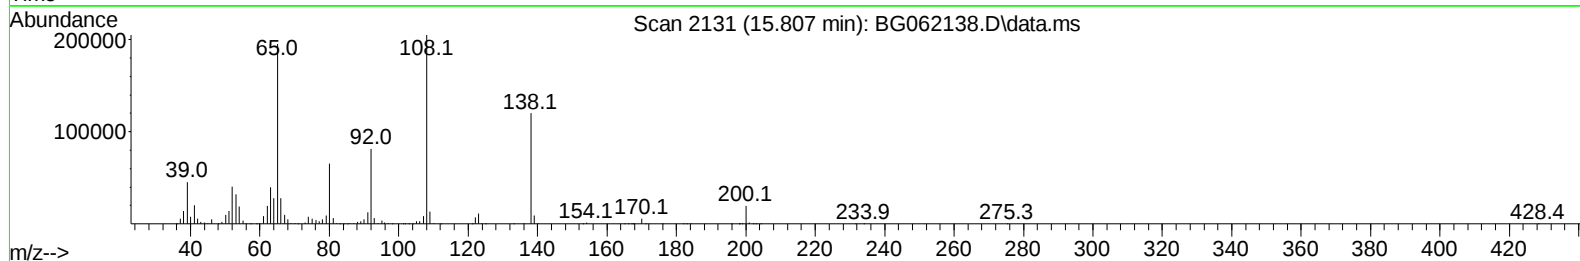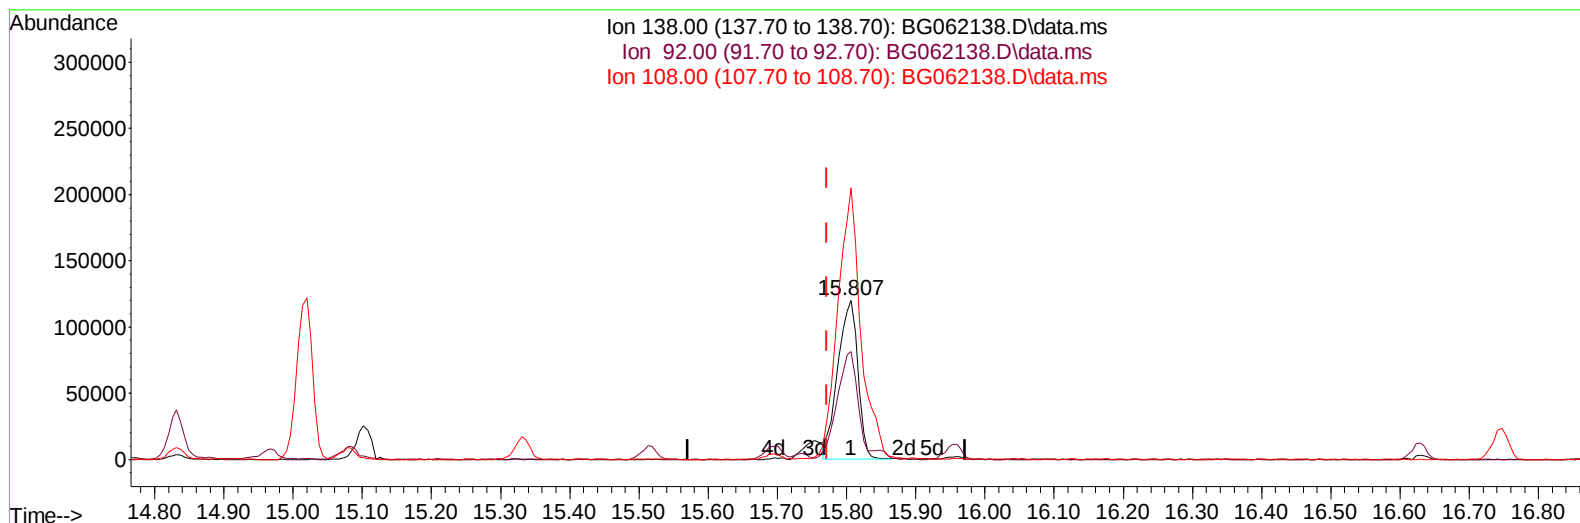

TIC: BG062138.D\data.ms

(63) 4-Nitroaniline

15.807min (+ 0.036) 132.66 ng/ul

response 242016

Ion	Exp%	Act%
138.00	100.00	100.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Quant Time: Jul 19 13:11:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

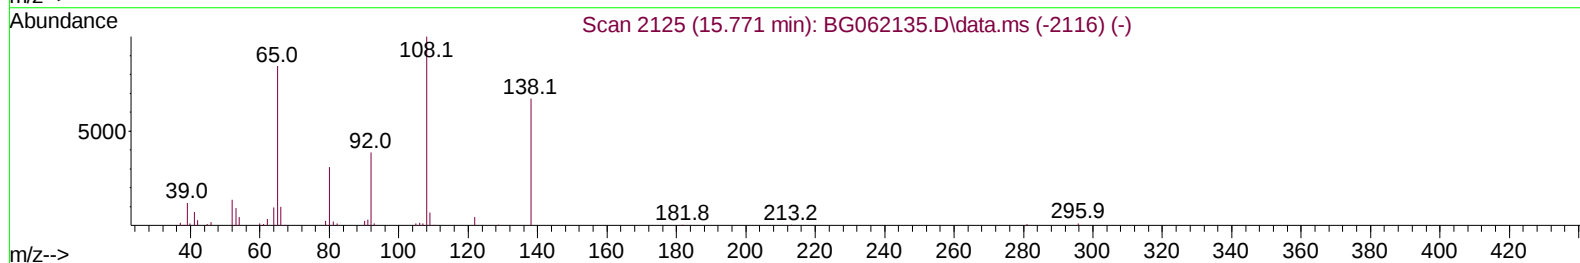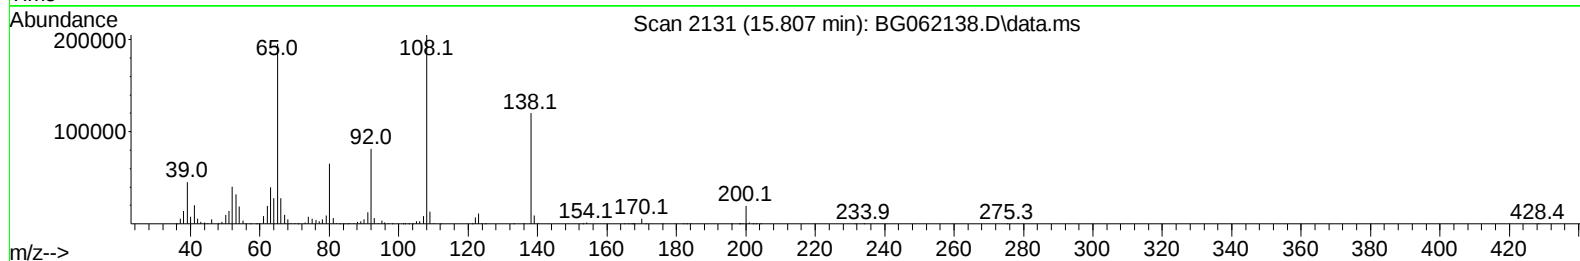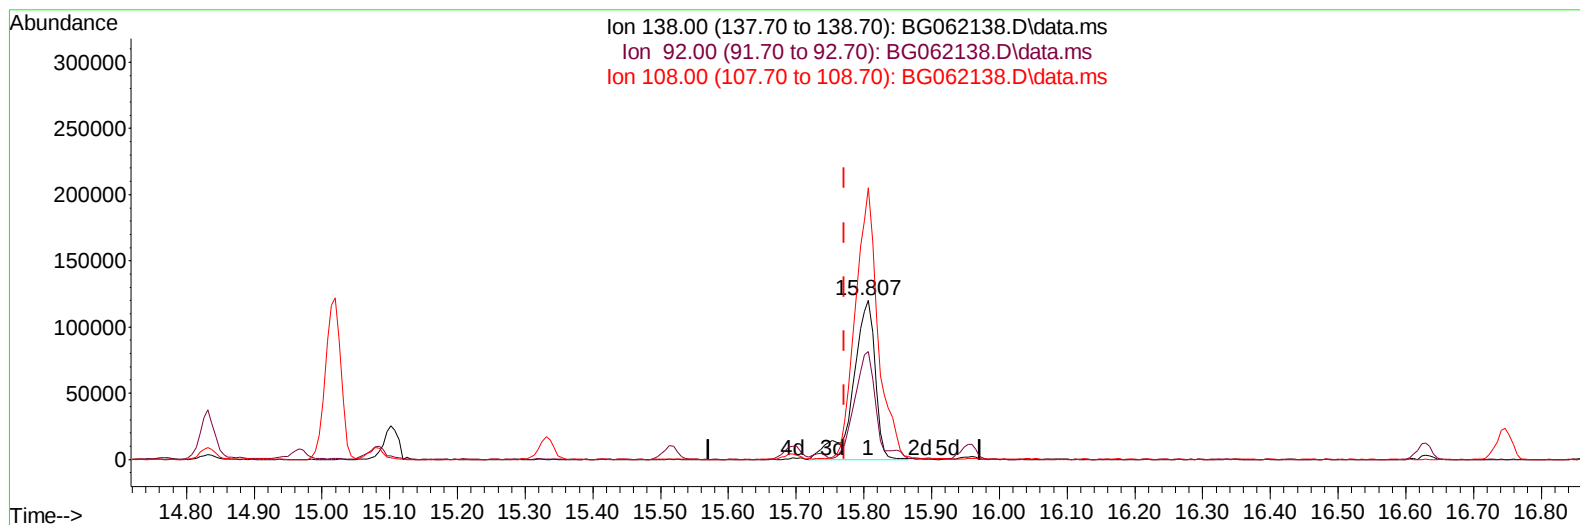

TIC: BG062138.D\data.ms

(63) 4-Nitroaniline

15.807min (+ 0.036) 148.24 ng/ul m

response 270437

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	58.80	67.90
108.00	148.80	170.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
 Data File : BG062138.D
 Acq On : 19 Jul 2024 12:37
 Operator : MA/JU
 Sample : SSTD16027
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD160409

Manual IntegrationsAPPROVED

Quant Time: Jul 19 13:17:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 19 12:42:00 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2024
 Supervised By :mohammad ahmed 07/23/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.070	152	36214	20.000	ng/ul	0.00
20) Naphthalene-d8	10.884	136	161909	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.702	164	132302	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.446	188	355305	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.716	240	360043	20.000	ng/ul	0.01
88) Perylene-d12	24.947	264	370720	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	3.876	84	471856	141.053	ng/ul	0.00
7) Phenol-d5	7.254	99	603119	154.799	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.395	67	332159	150.888	ng/ul	0.00
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	8.810	113	470084	162.802	ng/ul	0.02
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.00					

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

Quant Time: Jul 19 13:17:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062138.D
Acq On : 19 Jul 2024 12:37
Operator : MA/JU
Sample : SSTD16027
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD160409

Manual IntegrationsAPPROVED

Quant Time: Jul 19 13:17:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 12:42:00 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2024
Supervised By :mohammad ahmed 07/23/2024

