

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
 Data File : BG062141.D
 Acq On : 19 Jul 2024 15:33
 Operator : MA/JU
 Sample : PB162078BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.454	25	28	35	rVB3	11831	18837	1.02%	0.119%
2	3.530	40	41	48	rVB3	4194	5153	0.28%	0.033%
3	3.612	54	55	58	rVB2	4428	3217	0.17%	0.020%
4	3.683	65	67	71	rBV3	2396	2610	0.14%	0.017%
5	3.876	96	100	111	rBV	142628	239249	12.91%	1.517%
6	4.211	153	157	160	rBV5	2320	3077	0.17%	0.020%
7	4.458	196	199	200	rBV2	3437	2965	0.16%	0.019%
8	5.868	437	439	442	rBV2	2743	2718	0.15%	0.017%
9	6.632	564	569	571	rBV	1952	3554	0.19%	0.023%
10	7.237	666	672	681	rBV	191630	328686	17.73%	2.085%
11	7.389	691	698	705	rVB	133976	216927	11.70%	1.376%
12	7.601	727	734	741	rBV	165393	284911	15.37%	1.807%
13	8.065	806	813	820	rVB	140317	234334	12.64%	1.486%
14	8.782	927	935	945	rBV2	222560	401529	21.66%	2.547%
15	9.234	1004	1012	1020	rBV	192696	333783	18.01%	2.117%
16	9.956	1128	1135	1145	rBV	176354	311435	16.80%	1.975%
17	10.503	1221	1228	1240	rBV	272402	495110	26.71%	3.140%
18	10.879	1285	1292	1300	rBV	198455	352547	19.02%	2.236%
19	11.020	1306	1316	1325	rBV	212377	409127	22.07%	2.595%
20	12.101	1495	1500	1502	rBV	1968	2771	0.15%	0.018%
21	12.453	1557	1560	1566	rBV2	4060	6171	0.33%	0.039%
22	12.588	1578	1583	1585	rBV	1763	2968	0.16%	0.019%
23	13.193	1682	1686	1690	rVB	1926	2770	0.15%	0.018%
24	13.616	1754	1758	1761	rBV	2278	3010	0.16%	0.019%
25	13.716	1773	1775	1780	rVB	2634	2868	0.15%	0.018%
26	14.098	1833	1840	1847	rBV	554056	801743	43.25%	5.085%
27	14.392	1882	1890	1897	rBV2	505332	801448	43.24%	5.083%
28	14.586	1920	1923	1928	rBV	1739	2599	0.14%	0.016%
29	14.697	1933	1942	1951	rVB	368413	567783	30.63%	3.601%
30	14.920	1972	1980	1989	rBV	215650	365507	19.72%	2.318%
31	15.196	2024	2027	2030	rBV3	2719	3391	0.18%	0.022%
32	15.384	2056	2059	2062	rVB	2126	2567	0.14%	0.016%
33	15.508	2076	2080	2083	rVB	1502	2488	0.13%	0.016%
34	15.684	2104	2110	2117	rVB	686968	1069436	57.70%	6.783%
35	15.807	2125	2131	2143	rBV2	282593	421484	22.74%	2.673%
36	15.913	2148	2149	2152	rBV3	2479	2870	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
 Data File : BG062141.D
 Acq On : 19 Jul 2024 15:33
 Operator : MA/JU
 Sample : PB162078BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

37	16.148	2186	2189	2191	rVB	2488	2518	0.14%	0.016%
38	16.371	2226	2227	2231	rBV	2454	3368	0.18%	0.021%
39	16.577	2258	2262	2265	rBV	2075	3300	0.18%	0.021%
40	16.900	2316	2317	2321	rBV	3127	3444	0.19%	0.022%
41	17.440	2402	2409	2417	rBV	566178	853338	46.04%	5.412%
42	17.540	2419	2426	2434	rBV2	892453	1325128	71.49%	8.405%
43	18.081	2516	2518	2526	rVB4	6666	9490	0.51%	0.060%
44	18.586	2602	2604	2606	rBV3	3275	3010	0.16%	0.019%
45	18.692	2619	2622	2625	rBV3	3661	5387	0.29%	0.034%
46	18.803	2639	2641	2644	rBV	2619	2638	0.14%	0.017%
47	18.968	2667	2669	2673	rBV3	3358	4179	0.23%	0.027%
48	19.044	2680	2682	2683	rBV2	4601	3454	0.19%	0.022%
49	19.138	2696	2698	2699	rBV2	2878	2513	0.14%	0.016%
50	19.379	2736	2739	2746	rVB4	14543	23551	1.27%	0.149%
51	19.455	2750	2752	2757	rVB3	11208	15086	0.81%	0.096%
52	19.538	2764	2766	2768	rBV3	4414	3485	0.19%	0.022%
53	19.820	2808	2814	2822	rBV	1280541	1853534	100.00%	11.756%
54	21.699	3128	3134	3145	rVB2	662802	1083831	58.47%	6.874%
55	24.713	3638	3647	3660	rVB2	612993	1725777	93.11%	10.946%
56	24.936	3674	3685	3697	rVB	383968	1119196	60.38%	7.099%
57	29.800	4511	4513	4514	rBV2	12362	8490	0.46%	0.054%




Sum of corrected areas: 15766360

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062141.D
Acq On : 19 Jul 2024 15:33
Operator : MA/JU
Sample : PB162078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

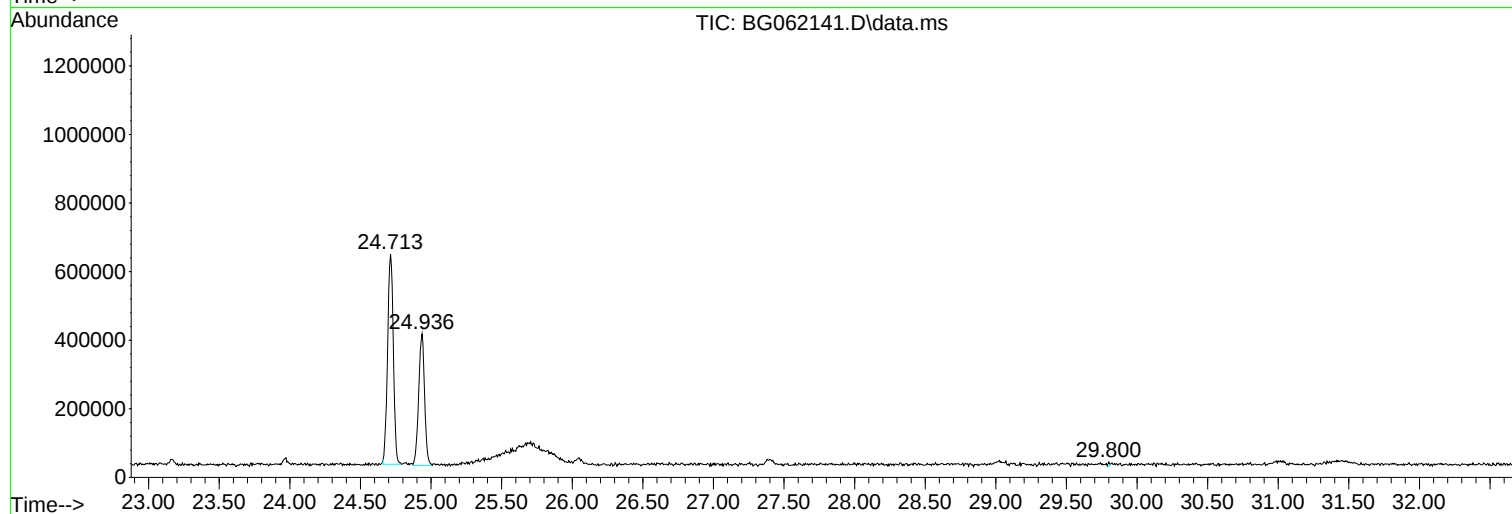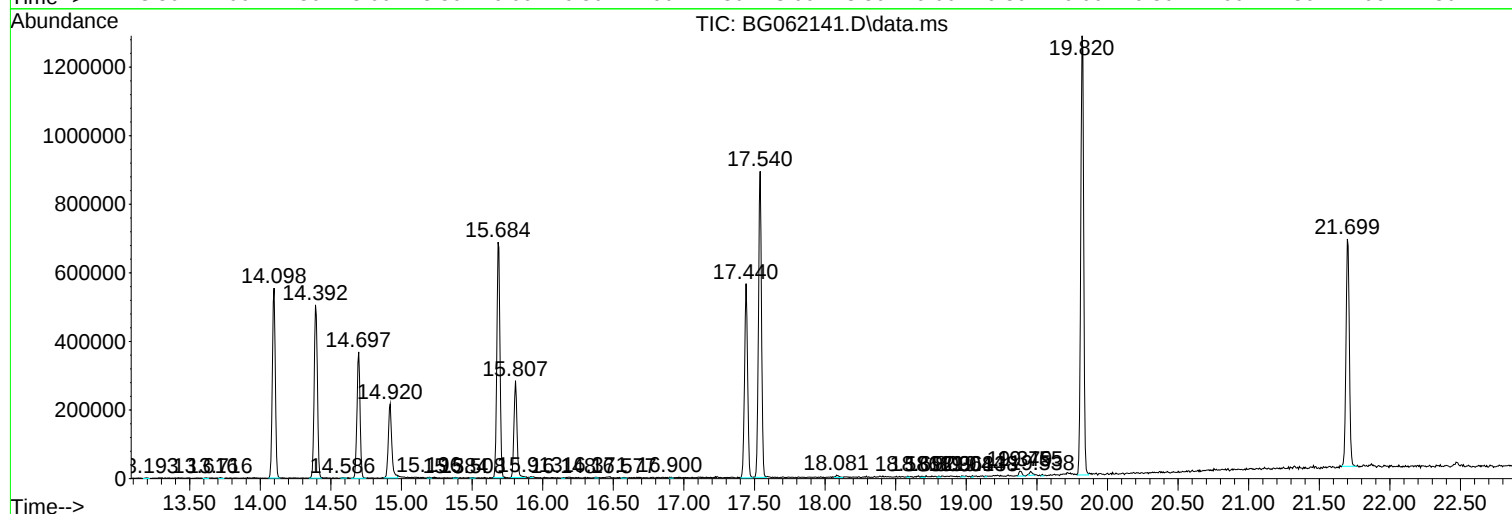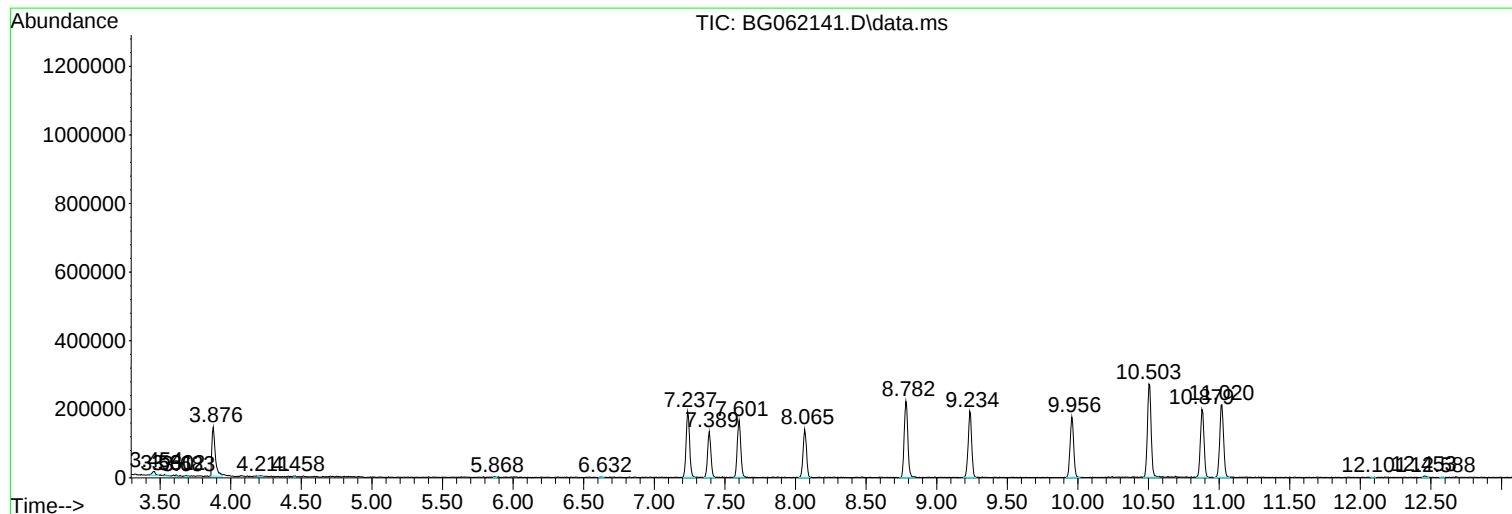

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062141.D
Acq On : 19 Jul 2024 15:33
Operator : MA/JU
Sample : PB162078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062141.D
Acq On : 19 Jul 2024 15:33
Operator : MA/JU
Sample : PB162078BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------