

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
 Data File : BG062145.D
 Acq On : 19 Jul 2024 18:16
 Operator : MA/JU
 Sample : P3237-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	25	28	34	rVB3	11640	17583	0.89%	0.108%
2	3.881	98	101	107	rBV	53588	83001	4.22%	0.508%
3	4.074	132	134	138	rBV2	1896	2877	0.15%	0.018%
4	4.157	143	148	149	rVV2	2859	3360	0.17%	0.021%
5	4.180	149	152	154	rVV2	3887	4137	0.21%	0.025%
6	4.210	154	157	162	rVV4	4492	7081	0.36%	0.043%
7	4.268	165	167	172	rVB2	2979	2901	0.15%	0.018%
8	4.638	227	230	235	rVB3	4705	8235	0.42%	0.050%
9	5.132	311	314	318	rVB3	5050	7766	0.39%	0.048%
10	7.241	667	673	682	rBV	65661	110007	5.59%	0.674%
11	7.388	692	698	704	rBV	133274	219342	11.15%	1.343%
12	7.599	725	734	742	rBV	175342	294718	14.98%	1.805%
13	8.063	807	813	820	rBV	154377	266518	13.54%	1.632%
14	8.786	929	936	943	rBV	165886	284301	14.45%	1.741%
15	9.232	1005	1012	1020	rBV	203227	361798	18.38%	2.216%
16	9.467	1050	1052	1057	rBV	2218	2925	0.15%	0.018%
17	9.955	1128	1135	1143	rBV2	187824	341394	17.35%	2.091%
18	10.196	1173	1176	1177	rBV	3249	2974	0.15%	0.018%
19	10.507	1222	1229	1236	rBV	273509	493692	25.09%	3.023%
20	10.877	1284	1292	1300	rVB	226703	410571	20.86%	2.514%
21	11.018	1308	1316	1323	rBV2	215308	396614	20.15%	2.429%
22	12.075	1494	1496	1501	rVB	2184	2933	0.15%	0.018%
23	12.457	1555	1561	1566	rVB3	7758	13585	0.69%	0.083%
24	12.675	1594	1598	1600	rVB	3085	3262	0.17%	0.020%
25	13.127	1672	1675	1677	rBV	2330	3348	0.17%	0.021%
26	13.497	1733	1738	1741	rBV2	4475	5920	0.30%	0.036%
27	13.773	1782	1785	1787	rBV2	2678	3245	0.16%	0.020%
28	14.096	1830	1840	1847	rBV	617989	889077	45.18%	5.444%
29	14.325	1876	1879	1881	rVB	2567	2821	0.14%	0.017%
30	14.390	1883	1890	1897	rVB	599860	935686	47.54%	5.730%
31	14.695	1935	1942	1949	rVB	437831	704989	35.82%	4.317%
32	14.919	1973	1980	1987	rBV2	67740	123255	6.26%	0.755%
33	15.048	1999	2002	2004	rBV2	3373	3701	0.19%	0.023%
34	15.236	2030	2034	2038	rBV3	2437	4612	0.23%	0.028%
35	15.418	2063	2065	2069	rVB3	4570	5301	0.27%	0.032%
36	15.471	2072	2074	2078	rVB2	4131	3764	0.19%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
 Data File : BG062145.D
 Acq On : 19 Jul 2024 18:16
 Operator : MA/JU
 Sample : P3237-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1GA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

37	15.682	2104	2110	2117	rBV	843884	1245173	63.27%	7.625%
38	15.806	2125	2131	2137	rBV	319173	470650	23.92%	2.882%
39	16.270	2208	2210	2213	rBV	3591	3049	0.15%	0.019%
40	16.370	2225	2227	2232	rBV4	3030	4856	0.25%	0.030%
41	16.546	2255	2257	2258	rBV	3567	2981	0.15%	0.018%
42	16.881	2311	2314	2315	rBV2	5035	3752	0.19%	0.023%
43	17.063	2343	2345	2348	rVB4	5124	3577	0.18%	0.022%
44	17.227	2370	2373	2375	rBV3	5192	7444	0.38%	0.046%
45	17.439	2402	2409	2416	rBV	714470	1044934	53.10%	6.399%
46	17.539	2419	2426	2436	rVB2	1018583	1547103	78.61%	9.474%
47	17.621	2438	2440	2442	rBV3	3609	4088	0.21%	0.025%
48	17.862	2480	2481	2484	rBV3	5840	3939	0.20%	0.024%
49	18.208	2538	2540	2541	rBV2	6046	4624	0.23%	0.028%
50	18.226	2541	2543	2545	rVB3	6798	4397	0.22%	0.027%
51	18.896	2656	2657	2658	rBV	6103	3249	0.17%	0.020%
52	19.818	2808	2814	2822	rVB	1361083	1968004	100.00%	12.051%
53	21.698	3128	3134	3140	rVB	711707	1132612	57.55%	6.936%
54	24.711	3637	3647	3658	rVB2	607290	1710043	86.89%	10.472%
55	24.929	3676	3684	3695	rVB	402909	1138426	57.85%	6.971%




Sum of corrected areas: 16330195

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062145.D
Acq On : 19 Jul 2024 18:16
Operator : MA/JU
Sample : P3237-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

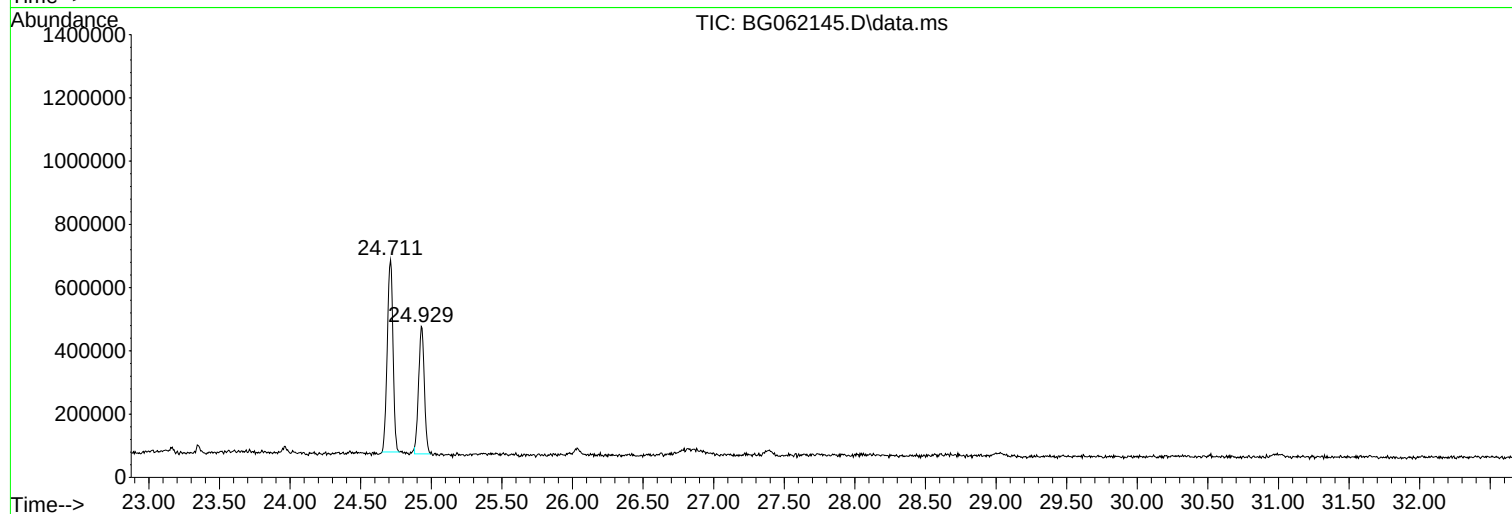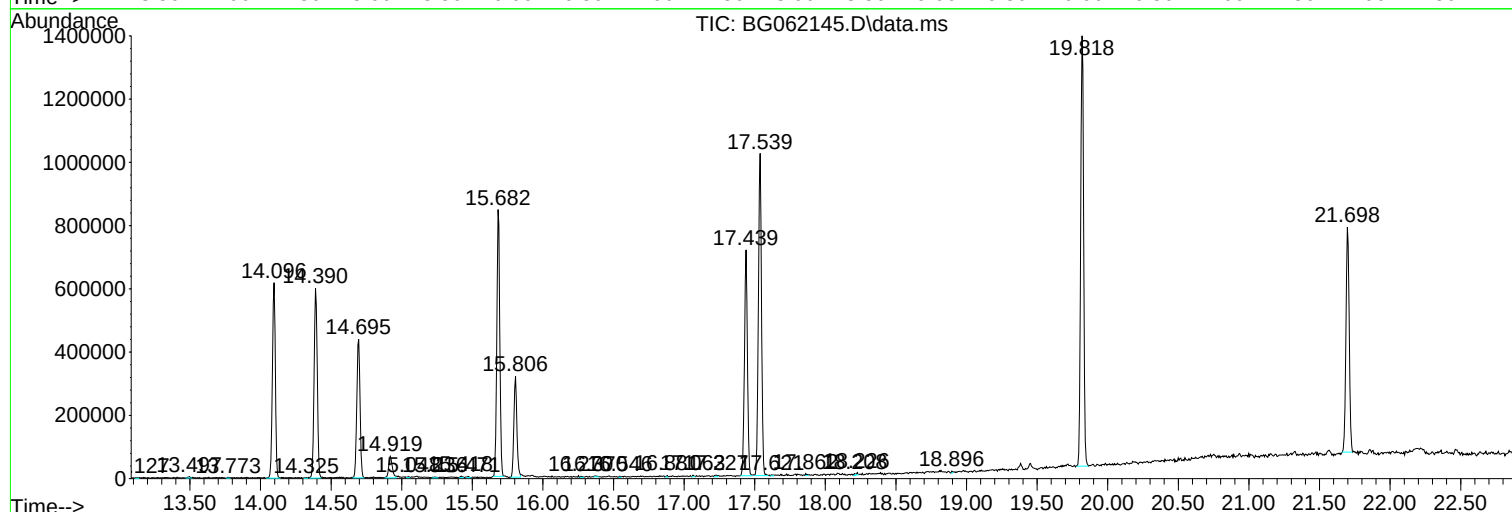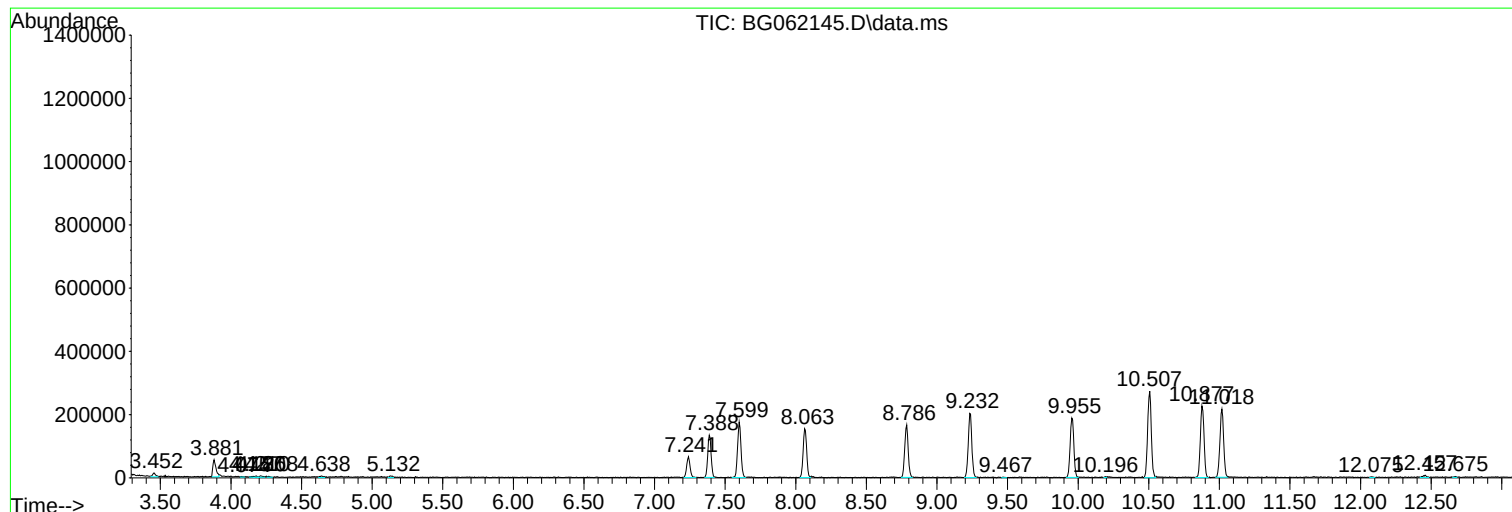

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062145.D
Acq On : 19 Jul 2024 18:16
Operator : MA/JU
Sample : P3237-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071924\
Data File : BG062145.D
Acq On : 19 Jul 2024 18:16
Operator : MA/JU
Sample : P3237-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1GA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc