
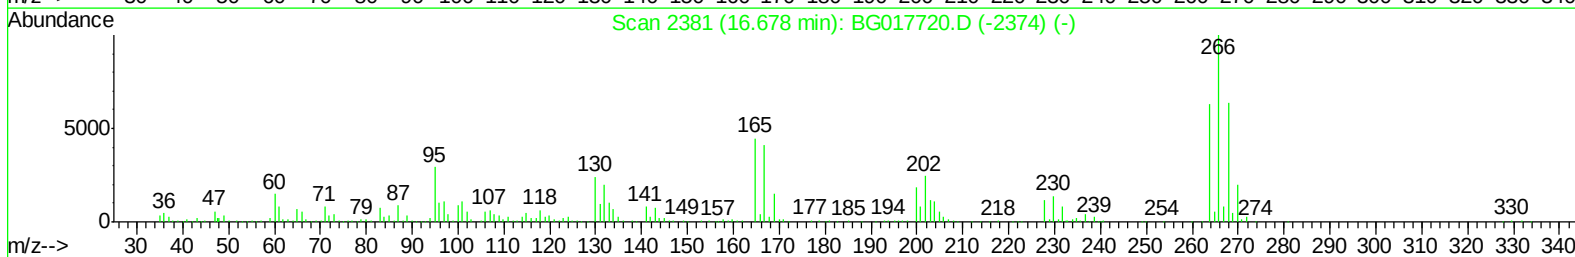
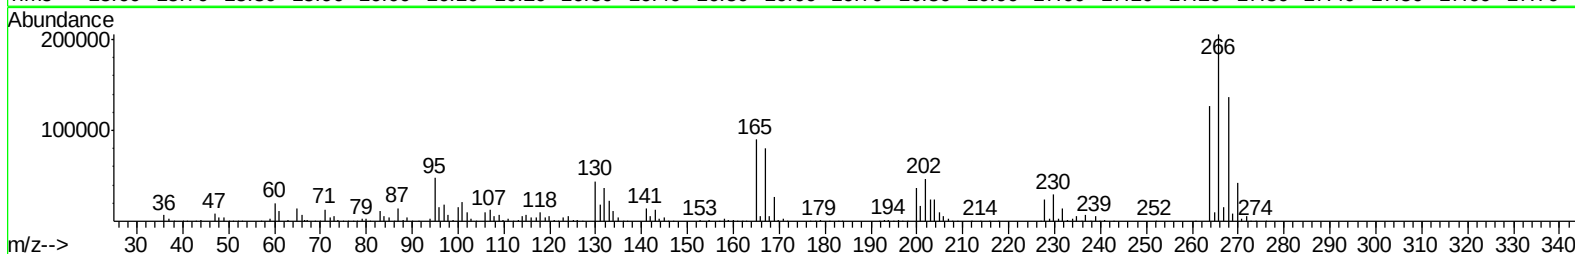


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
Data File : BG017981.D
Acq On : 20 Jul 2015 10:15
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 08:26:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 18 01:50:30 2015
Response via : Initial Calibration

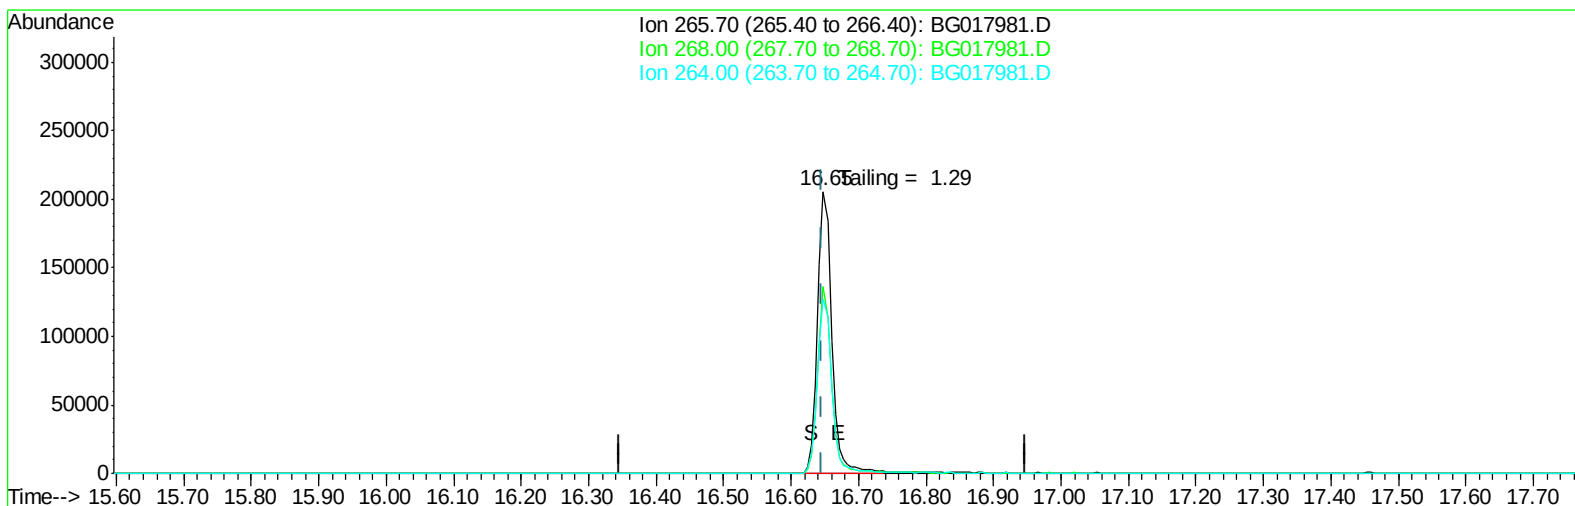

TIC: BG017981.D

(69) Pentachlorophenol (C)




16.648min (+0.001) 5417.86ng

response 296367

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	66.30
264.00	63.40	61.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
 Data File : BG017981.D
 Acq On : 20 Jul 2015 10:15
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 08:26:23 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 18 01:50:30 2015
 Response via : Initial Calibration

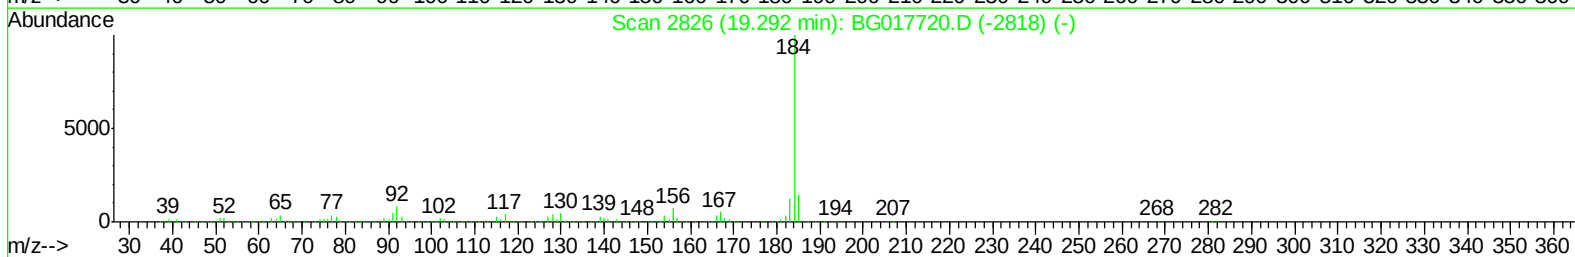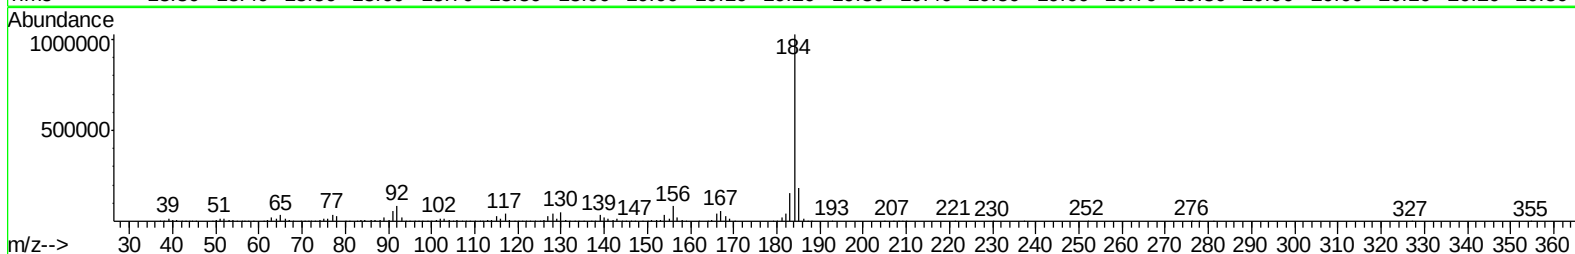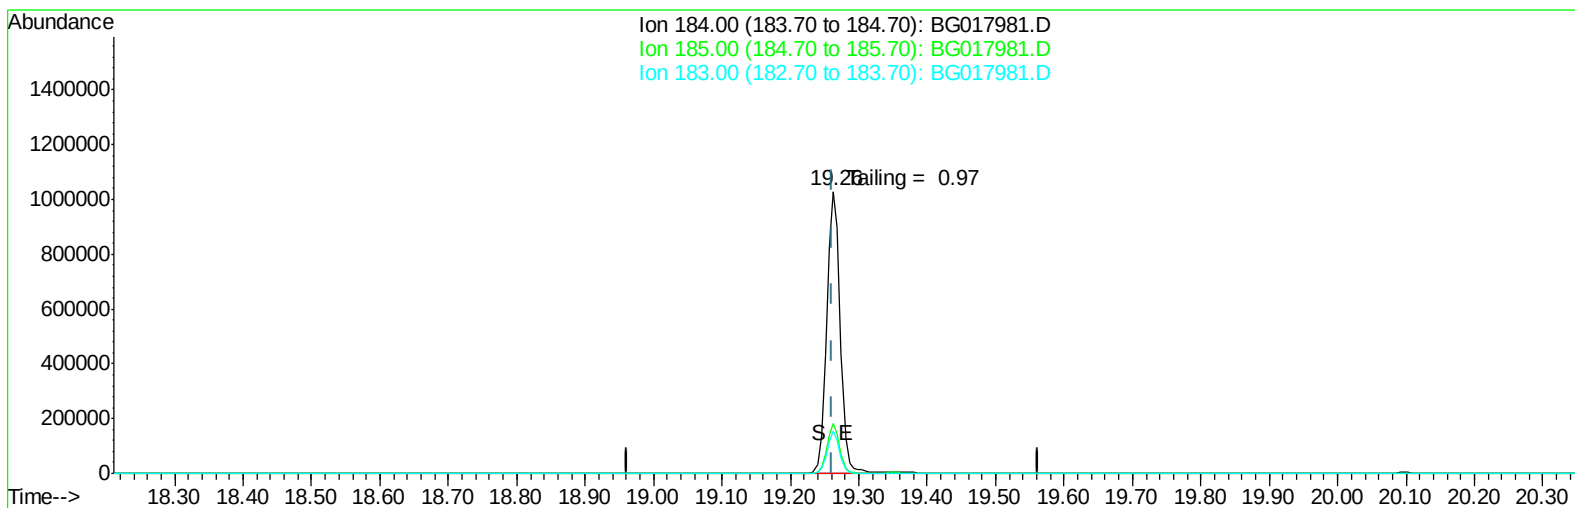

TIC: BG017981.D

(76) Benzidine

19.263min (+0.000) 95280.05ng

response 1428761

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	17.59#
183.00	12.50	14.80
0.00	0.00	0.00