

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
 Data File : BG017999.D
 Acq On : 20 Jul 2015 21:13
 Operator : TP/UM
 Sample : G3025-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 UST-2(0-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.604	150	156	167	rBV2	42843	88216	3.10%	0.172%
2	3.698	167	172	178	rBV2	47133	86256	3.03%	0.169%
3	3.845	190	197	205	rVV	91361	163467	5.74%	0.319%
4	3.944	208	214	221	rVB	46627	79548	2.79%	0.155%
5	4.744	344	350	356	rVV	138958	200370	7.04%	0.391%
6	5.131	411	416	421	rVB	54262	78713	2.77%	0.154%
7	5.202	421	428	434	rVV	1525766	2214027	77.78%	4.326%
8	5.261	434	438	455	rVB2	138187	395755	13.90%	0.773%
9	5.396	455	461	469	rBV	44486	73639	2.59%	0.144%
10	5.619	492	499	507	rVB2	50446	132616	4.66%	0.259%
11	5.883	538	544	551	rBV2	35538	73501	2.58%	0.144%
12	6.089	571	579	582	rBV4	43415	79765	2.80%	0.156%
13	6.588	655	664	671	rBV2	264320	541699	19.03%	1.058%
14	6.688	676	681	686	rVV	68617	111507	3.92%	0.218%
15	6.776	686	696	701	rVV	1518686	2475662	86.97%	4.837%
16	6.823	701	704	712	rVV2	79569	141096	4.96%	0.276%
17	7.129	748	756	763	rBV	1670991	2707310	95.11%	5.289%
18	7.241	770	775	781	rVB	231903	348392	12.24%	0.681%
19	7.587	828	834	841	rVB2	411676	705559	24.79%	1.378%
20	7.705	849	854	862	rVB2	48929	102374	3.60%	0.200%
21	7.816	862	873	881	rBV4	75107	203566	7.15%	0.398%
22	7.905	881	888	894	rVV	1165617	1904309	66.90%	3.720%
23	7.957	894	897	903	rVB	65057	90705	3.19%	0.177%
24	8.075	912	917	922	rBV2	121501	191220	6.72%	0.374%
25	8.128	922	926	937	rVB2	83966	162402	5.71%	0.317%
26	8.228	937	943	946	rBV2	131574	213875	7.51%	0.418%
27	8.257	946	948	955	rVB2	59466	97813	3.44%	0.191%
28	8.686	1015	1021	1025	rBV	181062	279670	9.83%	0.546%
29	8.745	1025	1031	1041	rVV	892755	1556185	54.67%	3.040%
30	9.209	1105	1110	1115	rVV	150797	243881	8.57%	0.476%
31	9.467	1147	1154	1159	rBV	47783	79228	2.78%	0.155%
32	9.620	1176	1180	1184	rVV	50947	83591	2.94%	0.163%
33	9.779	1201	1207	1214	rVB3	103058	206506	7.25%	0.403%
34	10.366	1298	1307	1312	rBV	544178	952978	33.48%	1.862%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
 Data File : BG017999.D
 Acq On : 20 Jul 2015 21:13
 Operator : TP/UM
 Sample : G3025-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 UST-2(0-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.413	1312	1315	1323	rVB	123842	202234	7.10%	0.395%
36	12.041	1585	1592	1600	rVB	116477	195158	6.86%	0.381%
37	12.264	1624	1630	1634	rBV	93560	148712	5.22%	0.291%
38	12.858	1723	1731	1738	rBV	1813210	2808995	98.68%	5.488%
39	13.404	1811	1824	1825	rBV3	73176	125877	4.42%	0.246%
40	13.563	1845	1851	1856	rBV2	119162	195245	6.86%	0.381%
41	13.616	1856	1860	1865	rVV	92810	126565	4.45%	0.247%
42	13.710	1870	1876	1885	rVV	819866	1171819	41.17%	2.289%
43	13.798	1885	1891	1895	rVV	76056	122302	4.30%	0.239%
44	13.962	1913	1919	1927	rBV3	49993	91015	3.20%	0.178%
45	14.244	1957	1967	1973	rBV2	767756	1256822	44.15%	2.455%
46	14.456	1998	2003	2012	rBV2	55870	153298	5.39%	0.299%
47	14.650	2027	2036	2042	rVB2	95245	190860	6.71%	0.373%
48	14.726	2042	2049	2053	rVB	99638	145443	5.11%	0.284%
49	14.791	2055	2060	2066	rBV7	37970	94044	3.30%	0.184%
50	14.873	2069	2074	2078	rVV	80770	149753	5.26%	0.293%
51	14.920	2078	2082	2087	rVB	78710	108136	3.80%	0.211%
52	15.037	2095	2102	2106	rBV2	73693	171043	6.01%	0.334%
53	15.078	2106	2109	2113	rVB3	58088	76399	2.68%	0.149%
54	15.296	2140	2146	2150	rBV3	114846	182054	6.40%	0.356%
55	15.519	2179	2184	2191	rBV5	85239	154054	5.41%	0.301%
56	15.596	2192	2197	2199	rBV3	53655	83438	2.93%	0.163%
57	15.742	2215	2222	2231	rVV	1791225	2527761	88.80%	4.938%
58	15.825	2231	2236	2247	rVB6	43568	131732	4.63%	0.257%
59	16.001	2258	2266	2273	rVB2	179078	384951	13.52%	0.752%
60	16.353	2322	2326	2330	rVB4	61923	85838	3.02%	0.168%
61	16.547	2350	2359	2360	rBV7	35482	80030	2.81%	0.156%
62	16.818	2401	2405	2415	rVB3	88739	187344	6.58%	0.366%
63	17.000	2430	2436	2439	rBV	834359	1169016	41.07%	2.284%
64	17.041	2439	2443	2449	rVB	942420	1250006	43.91%	2.442%
65	17.129	2454	2458	2463	rVB	195646	278327	9.78%	0.544%
66	17.405	2501	2505	2509	rBV2	71755	107889	3.79%	0.211%
67	17.875	2581	2585	2589	rBV	198149	255455	8.97%	0.499%
68	17.922	2589	2593	2600	rVV2	452191	717856	25.22%	1.402%
69	18.004	2604	2607	2612	rVV	104378	162525	5.71%	0.318%
70	18.069	2613	2618	2622	rVV2	282141	533765	18.75%	1.043%
71	18.110	2622	2625	2631	rVB	172137	259968	9.13%	0.508%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
Data File : BG017999.D
Acq On : 20 Jul 2015 21:13
Operator : TP/UM
Sample : G3025-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-2(0-2)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	18.386	2668	2672	2676	rVB	111792	125530	4.41%	0.245%
73	18.422	2676	2678	2684	rVB3	53433	75874	2.67%	0.148%
74	18.633	2711	2714	2718	rVB	85252	105352	3.70%	0.206%
75	18.780	2735	2739	2741	rBV2	161400	212529	7.47%	0.415%
76	18.868	2749	2754	2758	rBV5	49813	102906	3.62%	0.201%
77	18.945	2764	2767	2771	rBV	60298	98551	3.46%	0.193%
78	19.074	2783	2789	2793	rBV	1419716	1959578	68.84%	3.828%
79	19.133	2795	2799	2803	rVB2	335573	426430	14.98%	0.833%
80	19.209	2809	2812	2817	rBV6	76353	106435	3.74%	0.208%
81	19.432	2841	2850	2860	rBV	1391313	2327617	81.77%	4.547%
82	19.509	2860	2863	2870	rVB2	75160	149288	5.24%	0.292%
83	19.644	2882	2886	2891	rVB	2239242	2846499	100.00%	5.561%
84	19.767	2902	2907	2913	rBV2	96765	213927	7.52%	0.418%
85	19.855	2919	2922	2926	rBV	158531	191051	6.71%	0.373%
86	19.938	2932	2936	2940	rVB2	254775	338478	11.89%	0.661%
87	20.037	2949	2953	2957	rVB2	172227	219659	7.72%	0.429%
88	20.090	2958	2962	2967	rVB2	164137	216705	7.61%	0.423%
89	20.231	2983	2986	2989	rBV2	99801	110307	3.88%	0.216%
90	20.278	2991	2994	2995	rVV2	113507	142249	5.00%	0.278%
91	20.296	2995	2997	3003	rVB	225801	280460	9.85%	0.548%
92	20.889	3095	3098	3100	rBV	111470	115664	4.06%	0.226%
93	20.925	3100	3104	3110	rVV2	567487	709094	24.91%	1.385%
94	21.201	3144	3151	3155	rBV2	1283473	2553681	89.71%	4.989%
95	21.236	3155	3157	3167	rVB	690109	848954	29.82%	1.659%
96	21.353	3175	3177	3183	rVB2	98385	146724	5.15%	0.287%
97	22.758	3411	3416	3421	rBV2	440688	1010779	35.51%	1.975%
98	23.234	3493	3497	3503	rVB	280077	505731	17.77%	0.988%
99	23.328	3508	3513	3519	rVB	422542	786433	27.63%	1.536%
100	23.428	3524	3530	3535	rBV2	581545	1107538	38.91%	2.164%


Sum of corrected areas: 51185153

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
Data File : BG017999.D
Acq On : 20 Jul 2015 21:13
Operator : TP/UM
Sample : G3025-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-2(0-2)

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

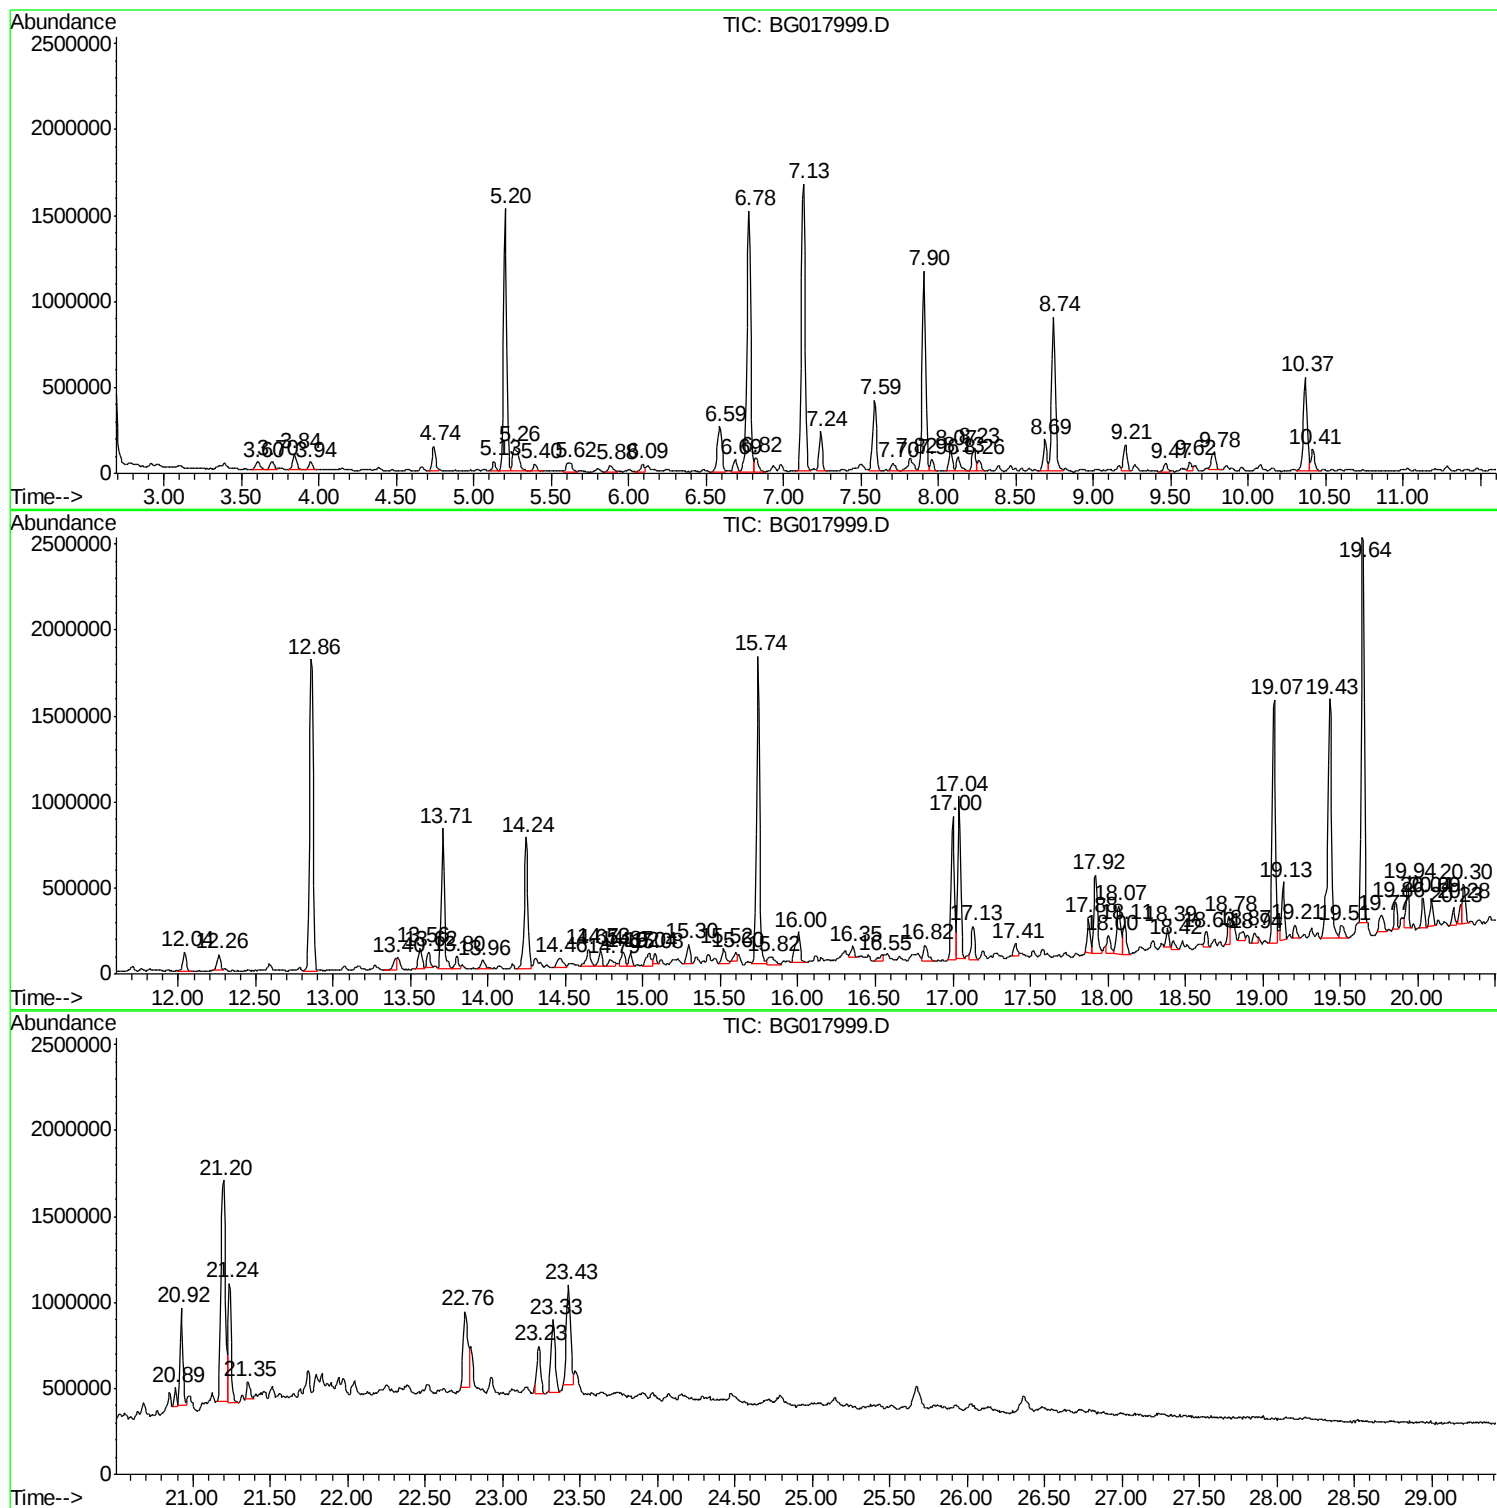

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
Data File : BG017999.D
Acq On : 20 Jul 2015 21:13
Operator : TP/UM
Sample : G3025-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-2(0-2)

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\Data\BG072015\
Data File : BG017999.D
Acq On : 20 Jul 2015 21:13
Operator : TP/UM
Sample : G3025-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-2(0-2)

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG071715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc