


Data Path : S:\HPCHEM1\BNA_G\DATA\BG072015\
 Data File : BG017981.D
 Acq On : 20 Jul 2015 10:15
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 06:05:07 2015

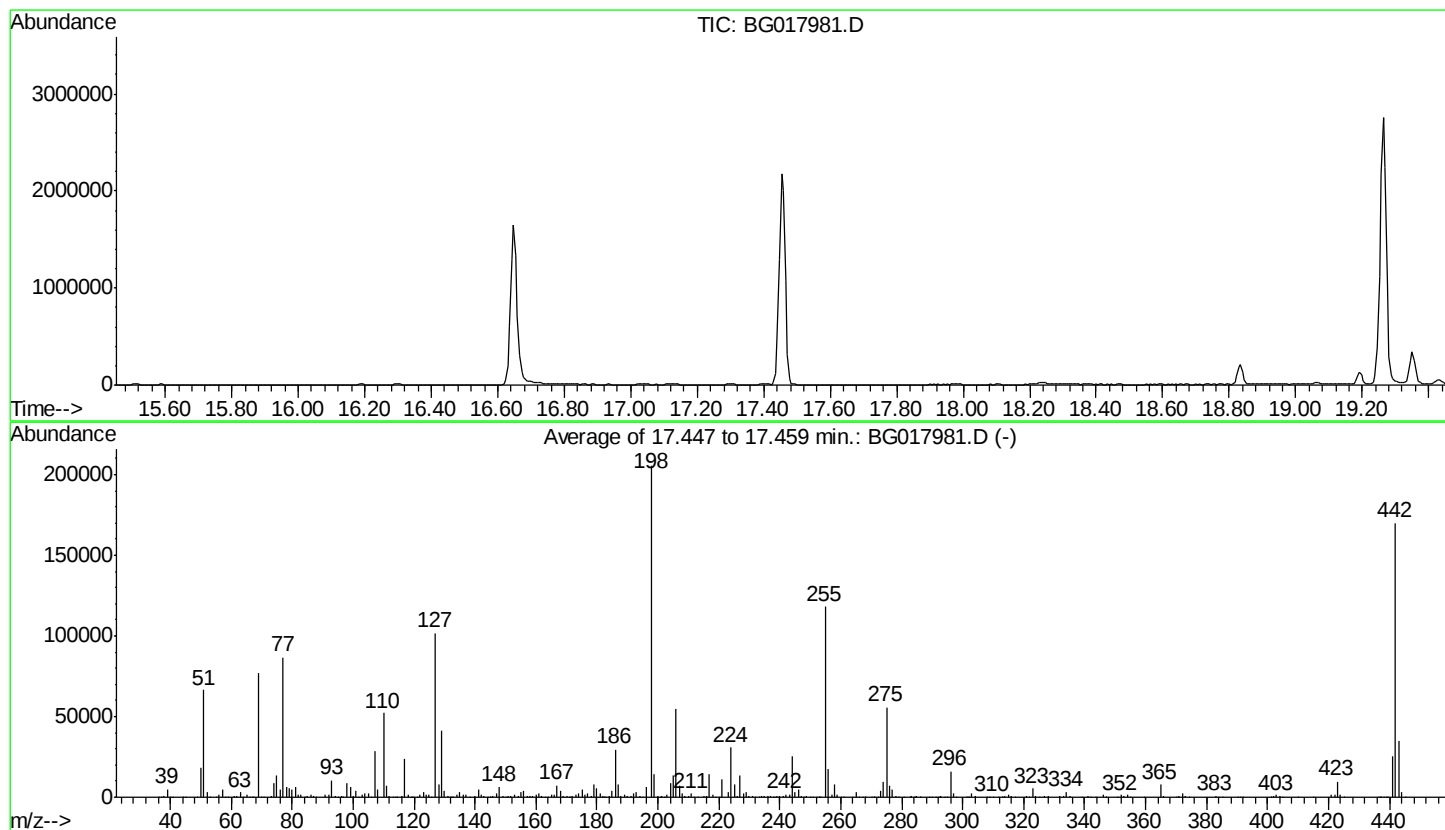

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	66625	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	77069	PASS
70	69	0.00	2	0.5	367	PASS
127	198	10	80	49.5	101762	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	205525	PASS
199	198	5	9	6.8	14002	PASS
275	198	10	60	27.1	55656	PASS
365	198	1	100	3.8	7765	PASS
441	442	0.01	24	14.7	25043	PASS
442	198	50	100	82.8	170088	PASS
443	442	15	24	20.5	34885	PASS