
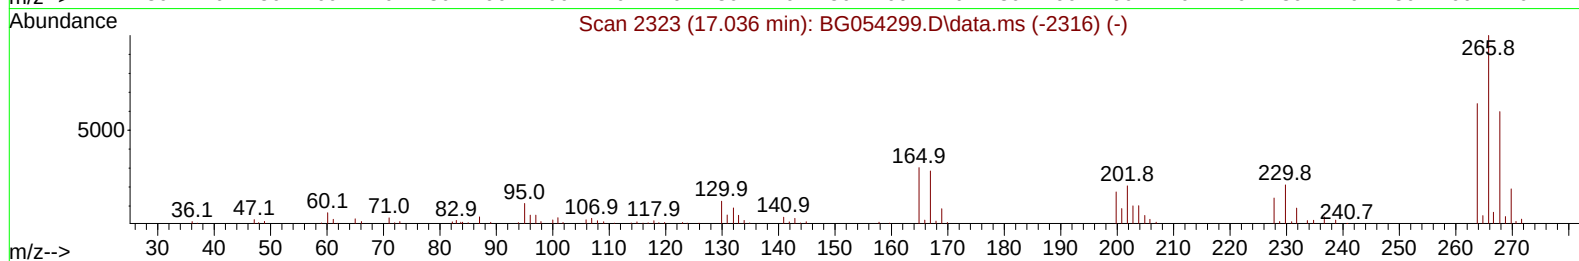
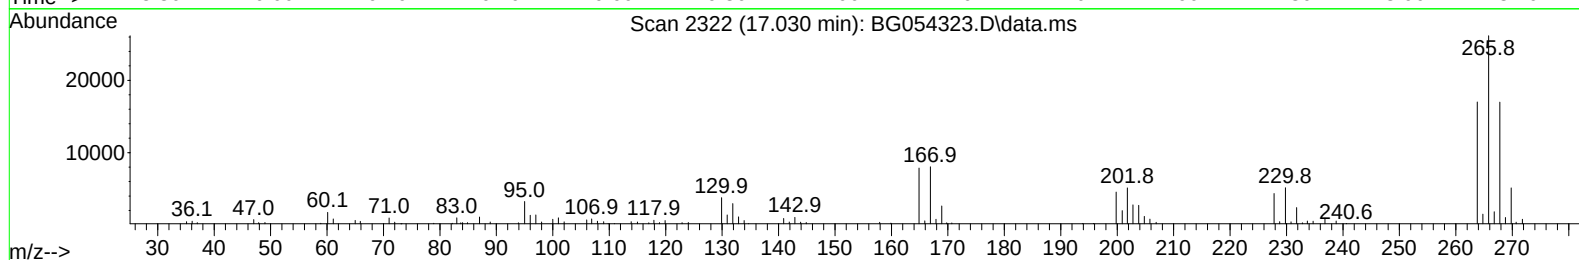


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072022\
Data File : BG054323.D
Acq On : 20 Jul 2022 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 02:55:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

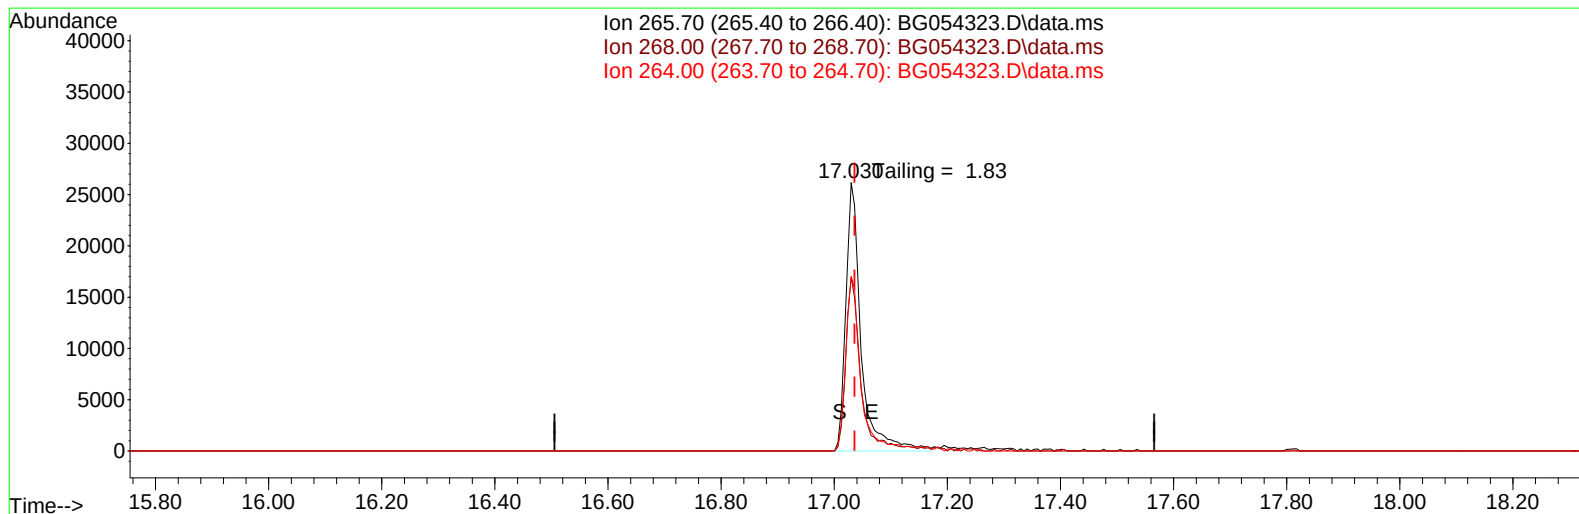

TIC: BG054323.D\data.ms

(70) Pentachlorophenol (C)




17.030min (-0.006) 20554.00 ng

response 48835

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.87
264.00	66.20	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072022\
Data File : BG054323.D
Acq On : 20 Jul 2022 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 02:55:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

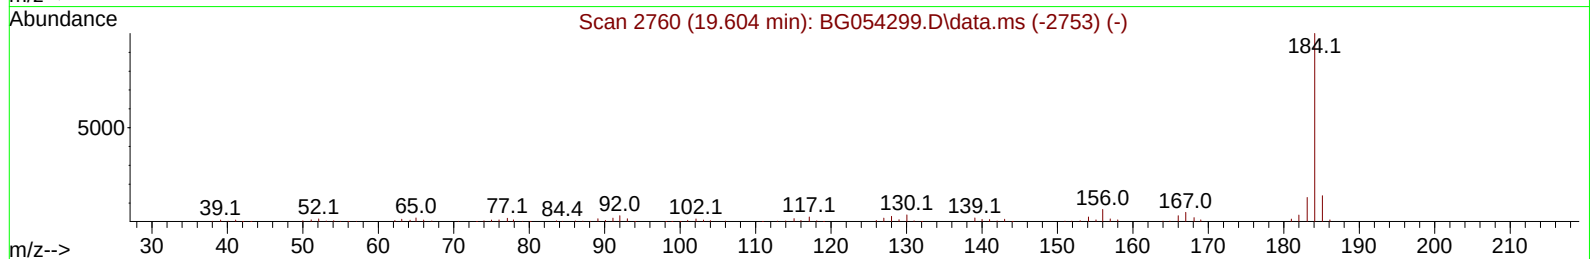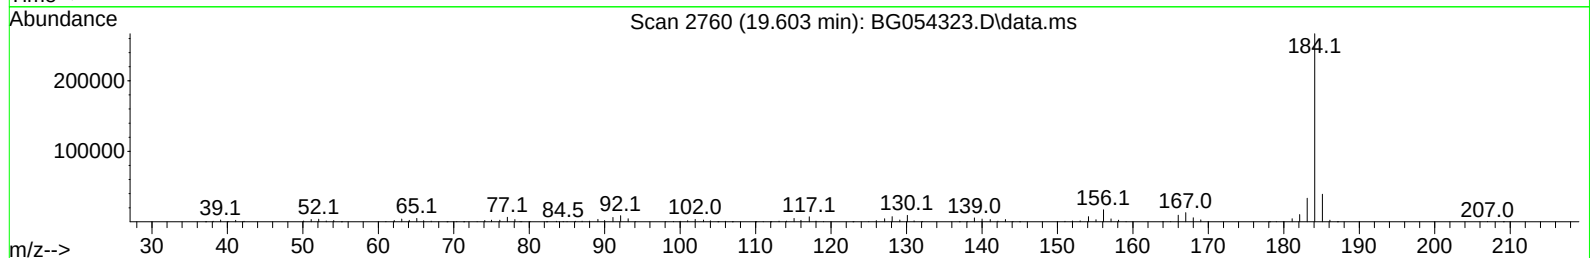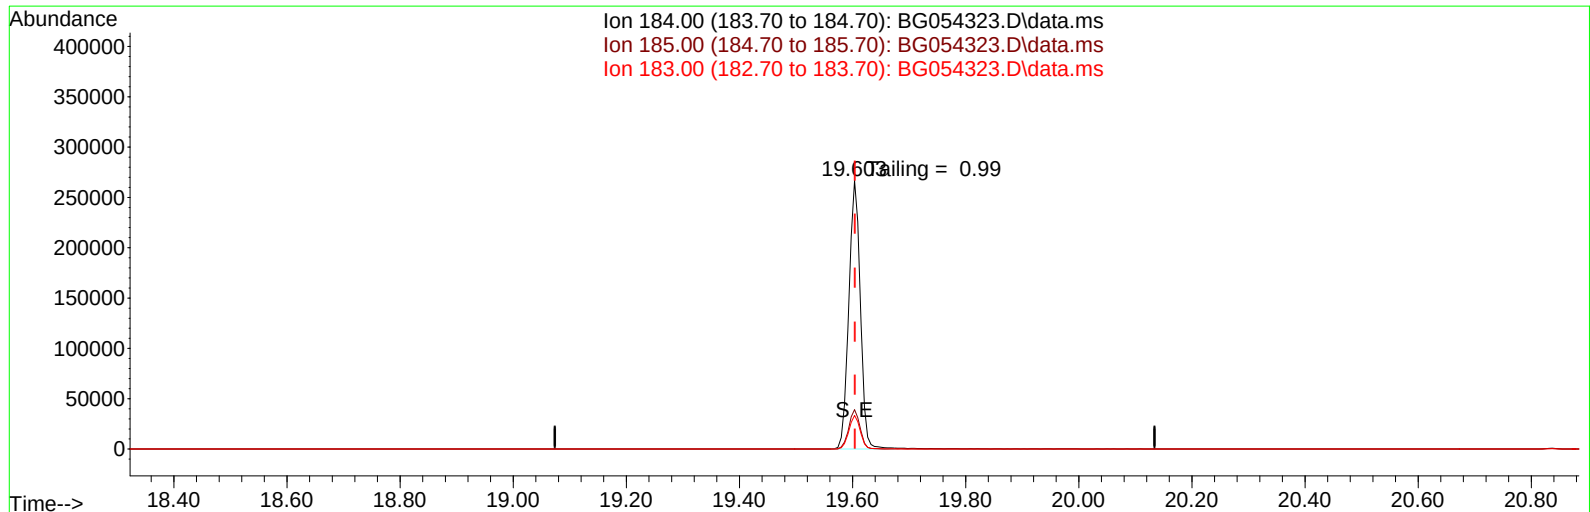

TIC: BG054323.D\data.ms

(77) Benzidine

19.603min (-0.001) 0.00 ng

response 380025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.67
183.00	11.10	12.53
0.00	0.00	0.00