


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072022\
 Data File : BG054323.D
 Acq On : 20 Jul 2022 11:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

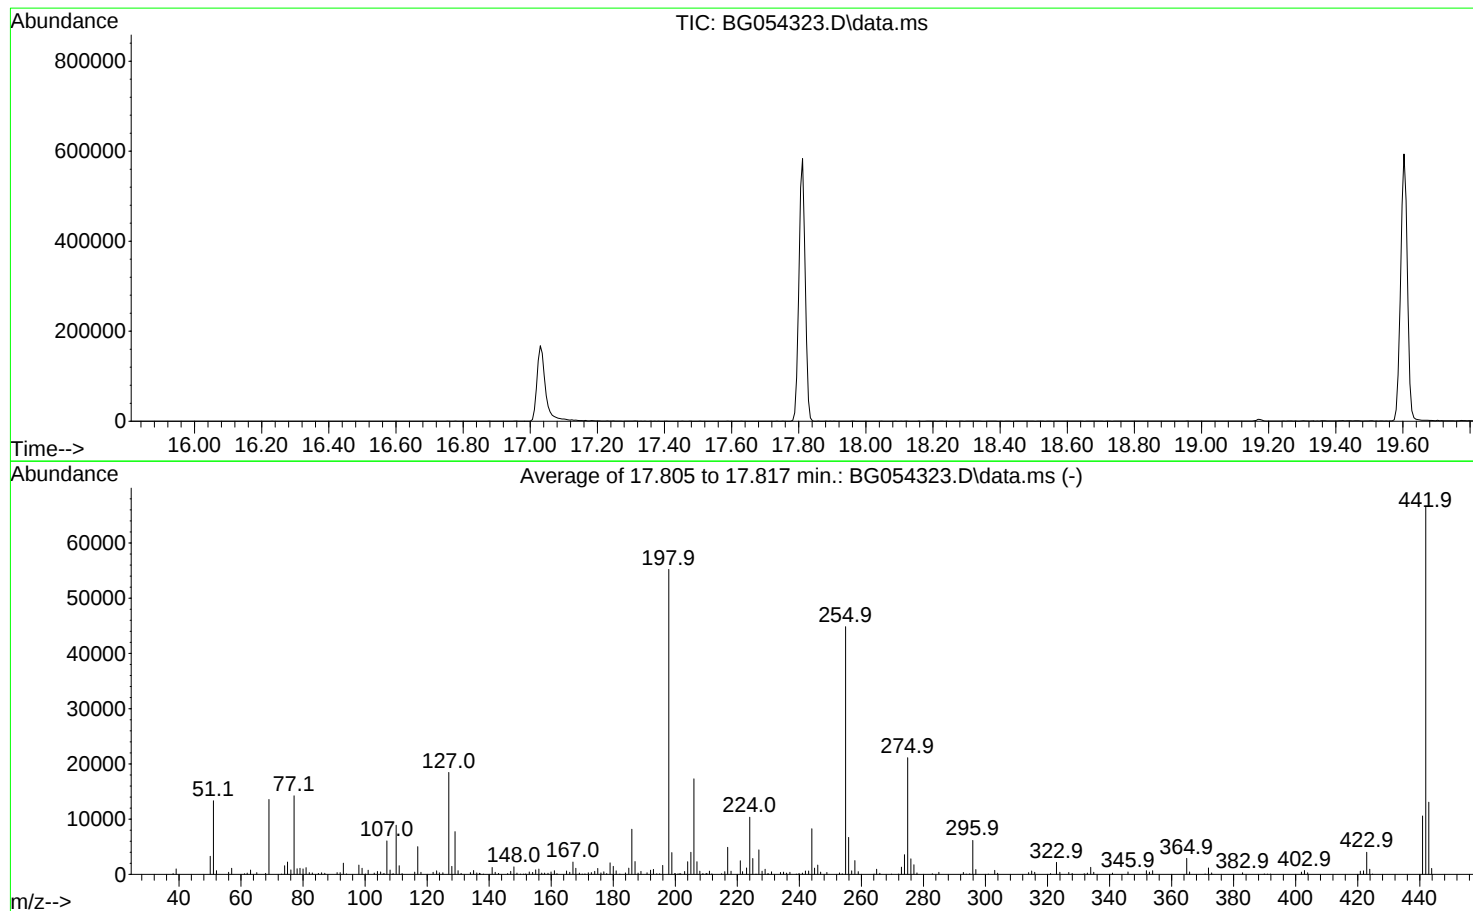

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	13325	PASS
68	69	0.00	2	1.3	176	PASS
69	198	0.00	100	24.6	13557	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.4	18454	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55211	PASS
199	198	5	9	7.2	3953	PASS
275	198	10	60	38.2	21109	PASS
365	198	1	100	5.2	2889	PASS
441	198	0.01	100	19.2	10576	PASS
442	442	50	100	100.0	66608	PASS
443	442	15	24	19.6	13069	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/20/2022	BNA_G	<u>BG054323.D</u>
Compound Name	Response	Retention Time
DDT	241033	20.837
DDD	4264	20.397
DDE	0	19.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4264	245297	1.74

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072022\
Data File : BG054323.D
Acq On : 20 Jul 2022 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 21 02:55:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

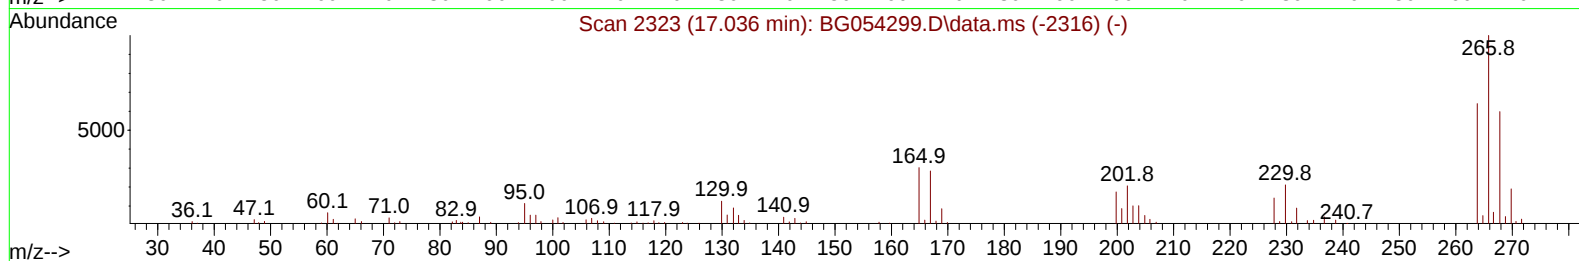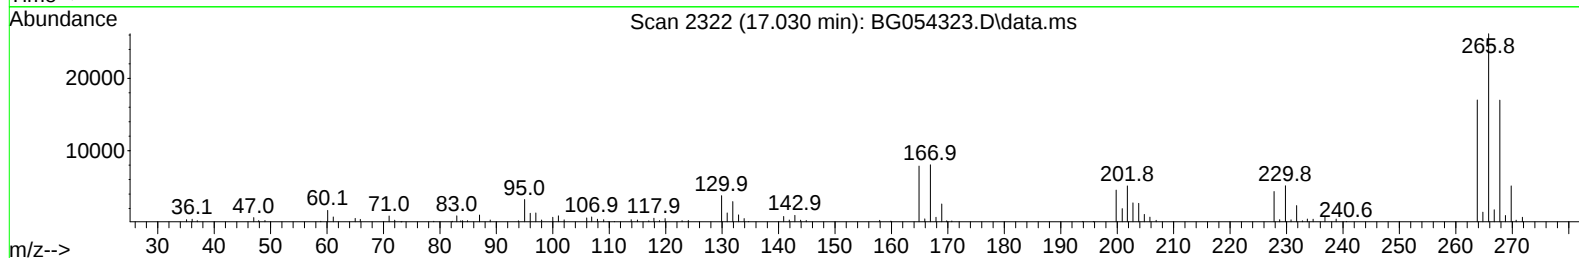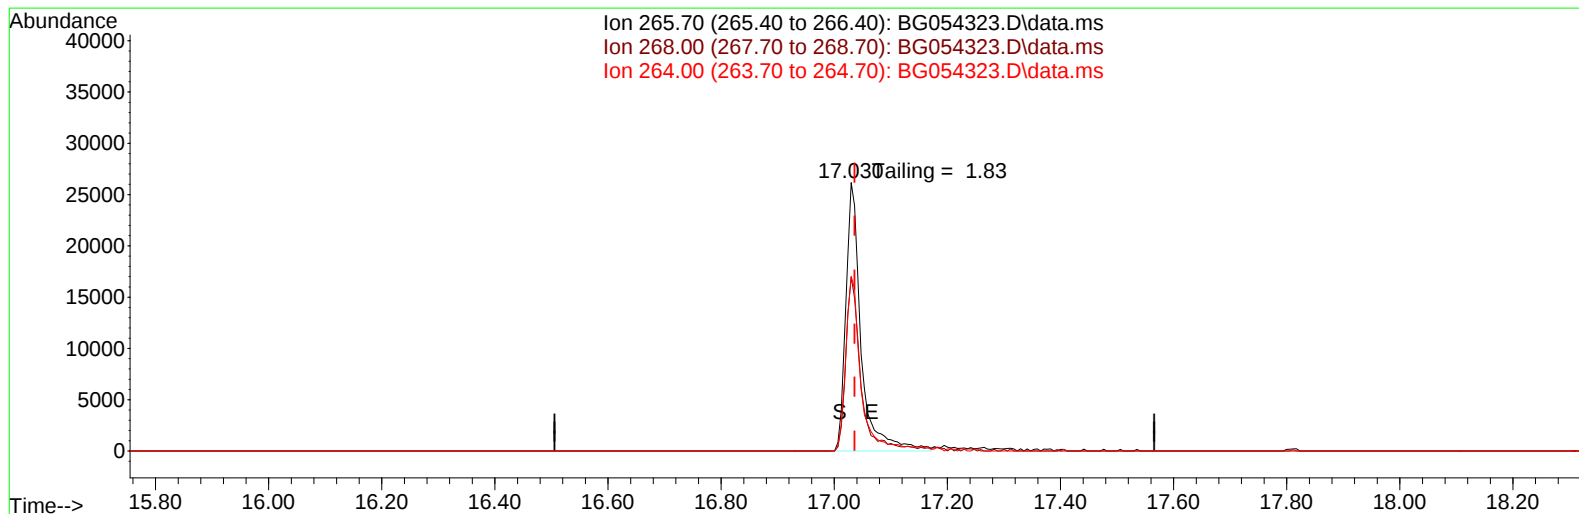

TIC: BG054323.D\data.ms

(70) Pentachlorophenol (C)

17.030min (-0.006) 20554.00 ng




response 48835

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.87
264.00	66.20	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072022\
Data File : BG054323.D
Acq On : 20 Jul 2022 11:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 21 02:55:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

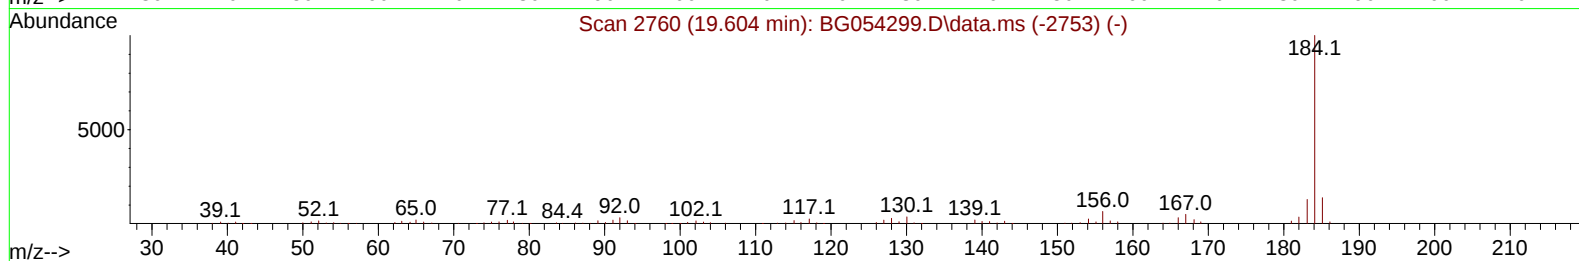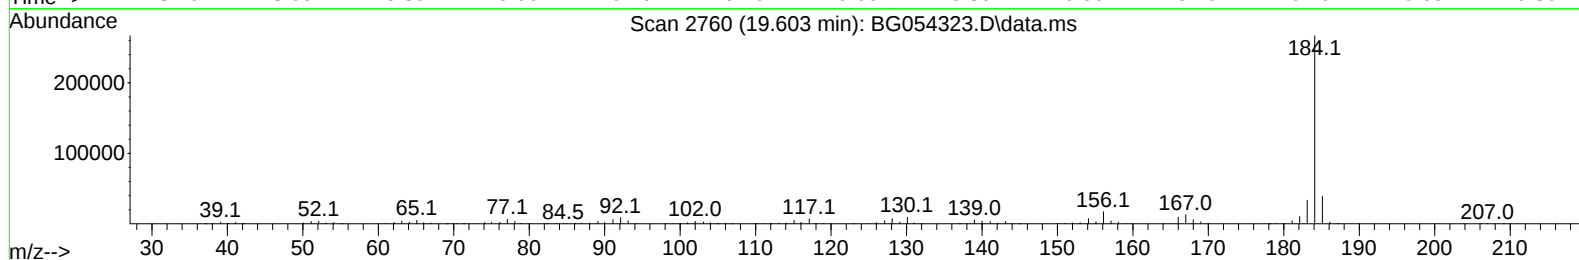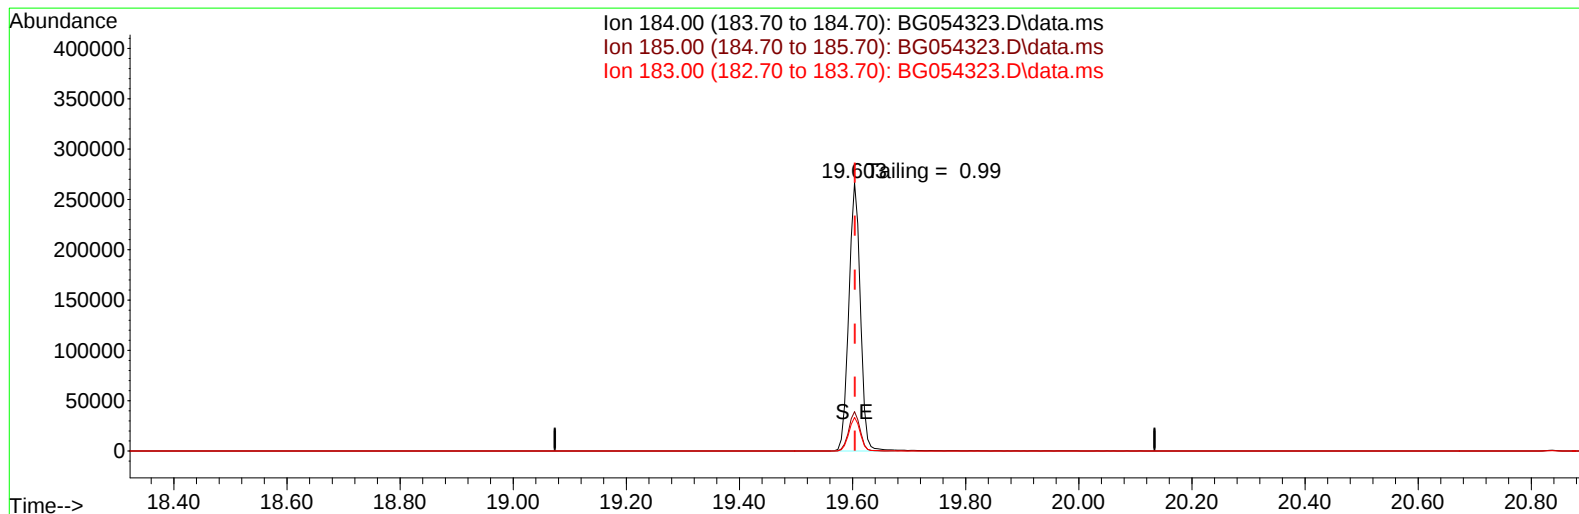

TIC: BG054323.D\data.ms

(77) Benzidine

19.603min (-0.001) 0.00 ng

response 380025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.67
183.00	11.10	12.53
0.00	0.00	0.00