


Data Path : Z:\HPCHEM1\BNA_G\Data\BG072115\
 Data File : BG018019.D
 Acq On : 21 Jul 2015 11:27
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 13 02:22:44 2015

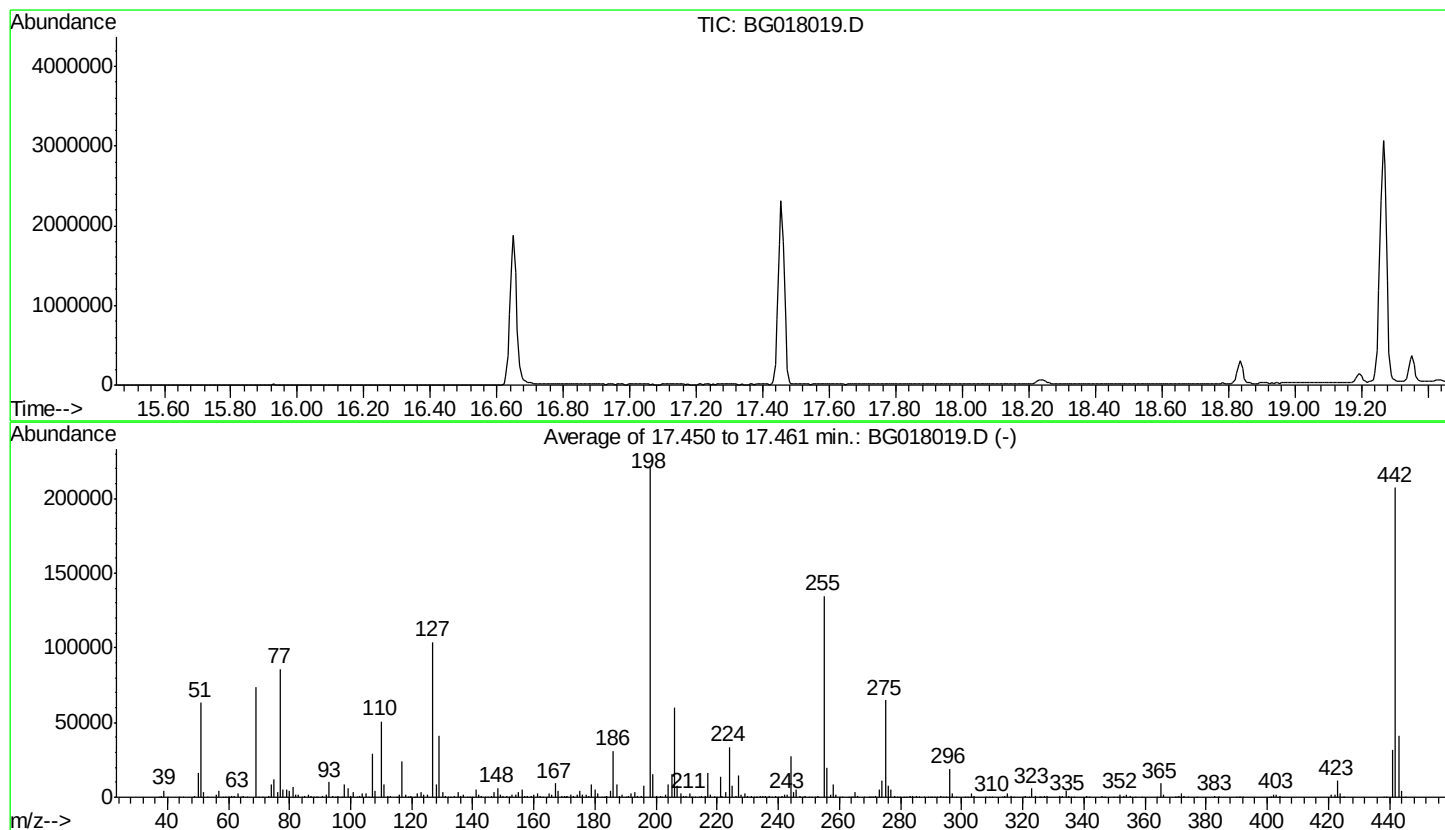

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	63058	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	73964	PASS
70	69	0.00	2	0.4	300	PASS
127	198	10	80	46.8	103888	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	221973	PASS
199	198	5	9	7.1	15706	PASS
275	198	10	60	29.2	64733	PASS
365	198	1	100	4.2	9396	PASS
441	442	0.01	24	15.2	31560	PASS
442	198	50	100	93.3	207104	PASS
443	442	15	24	19.8	40981	PASS