
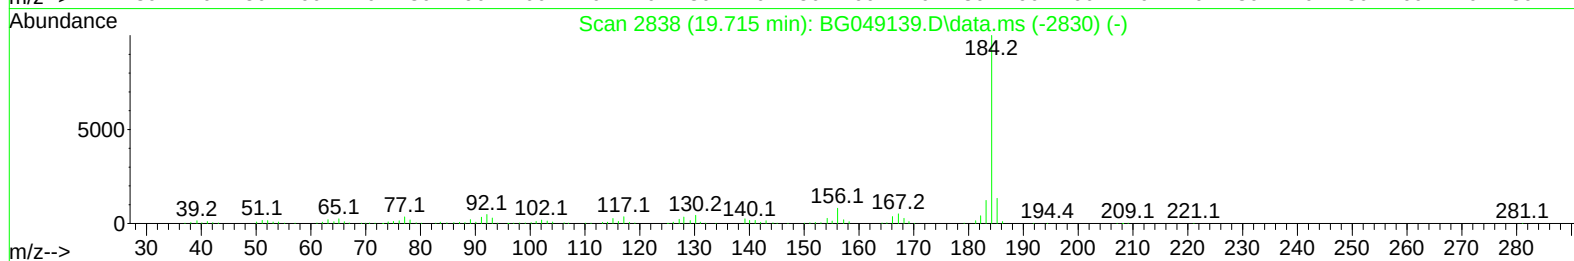
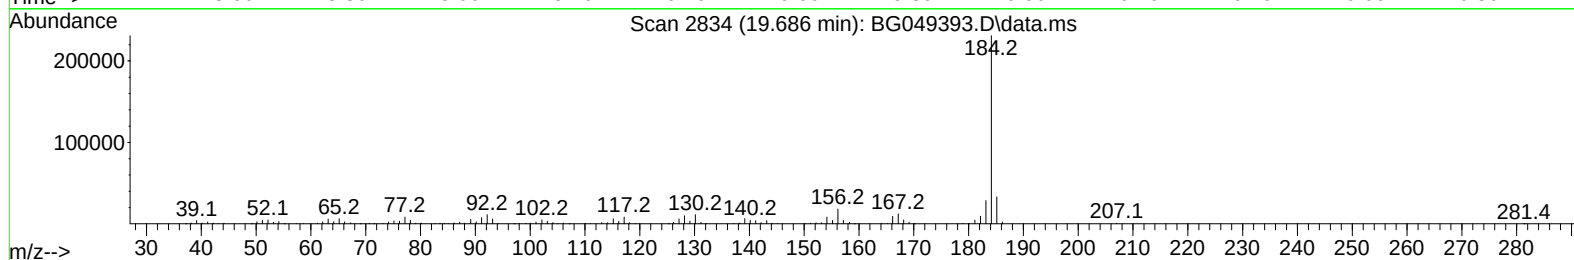


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072121\
Data File : BG049393.D
Acq On : 21 Jul 2021 10:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 12:53:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 11:36:30 2021
Response via : Initial Calibration

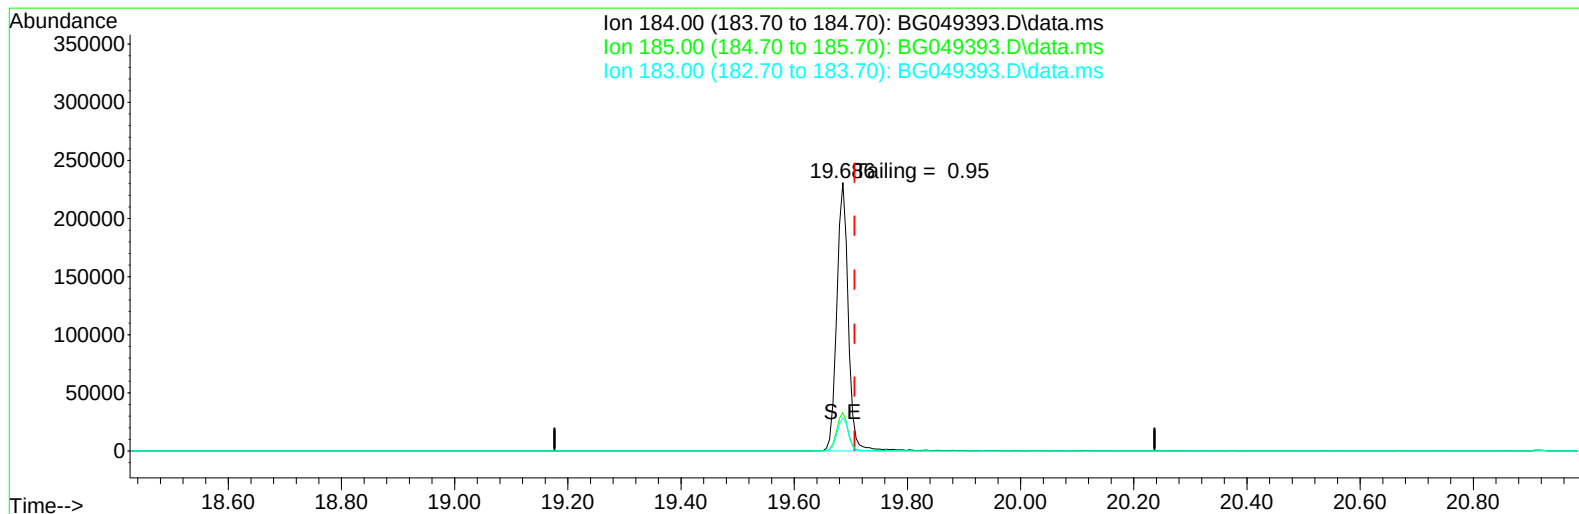

TIC: BG049393.D\data.ms

(77) Benzidine




19.686min (-0.020) 0.00 ng

response 321978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.38
183.00	11.70	12.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072121\
Data File : BG049393.D
Acq On : 21 Jul 2021 10:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 12:53:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 11:36:30 2021
Response via : Initial Calibration

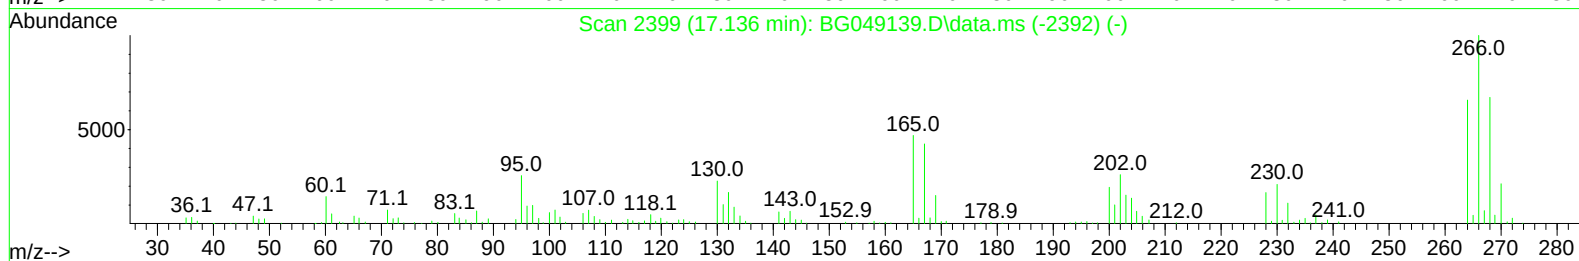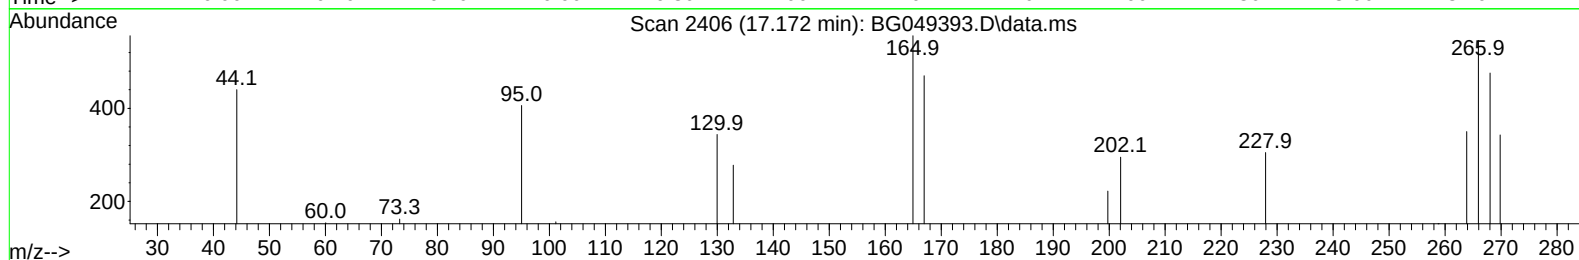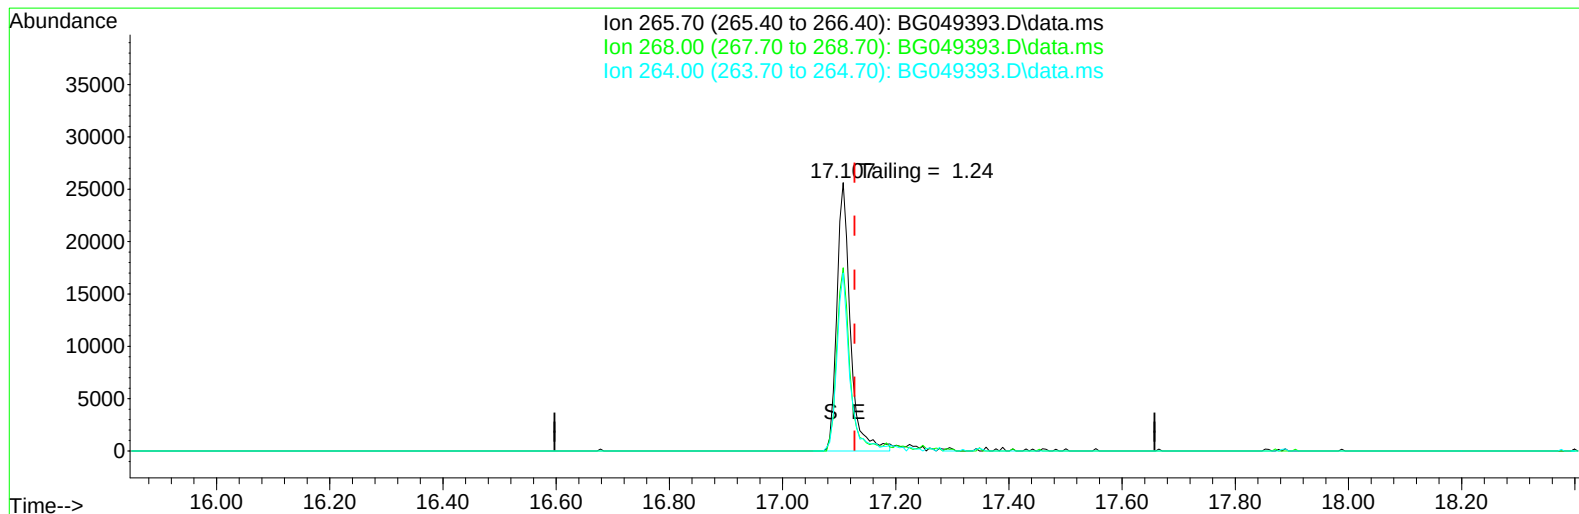

TIC: BG049393.D\data.ms

(70) Pentachlorophenol (C)

17.107min (-0.020) 22426.16 ng

response 41859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	68.26
264.00	61.30	66.35
0.00	0.00	0.00