
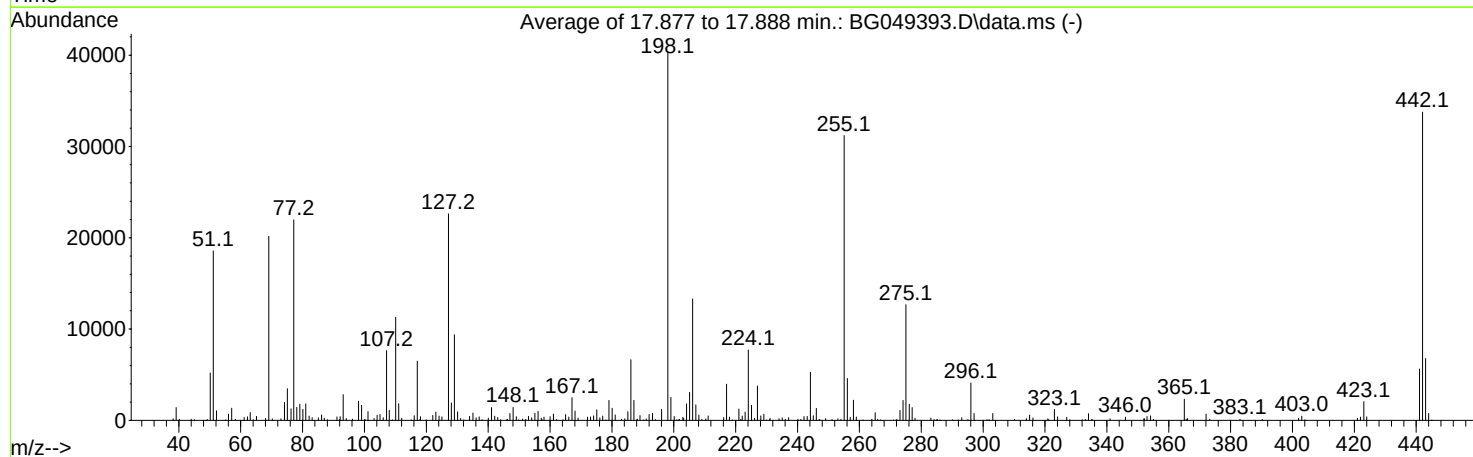


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072121\  
 Data File : BG049393.D  
 Acq On : 21 Jul 2021 10:37  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG072121.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jul 21 16:57:05 2021

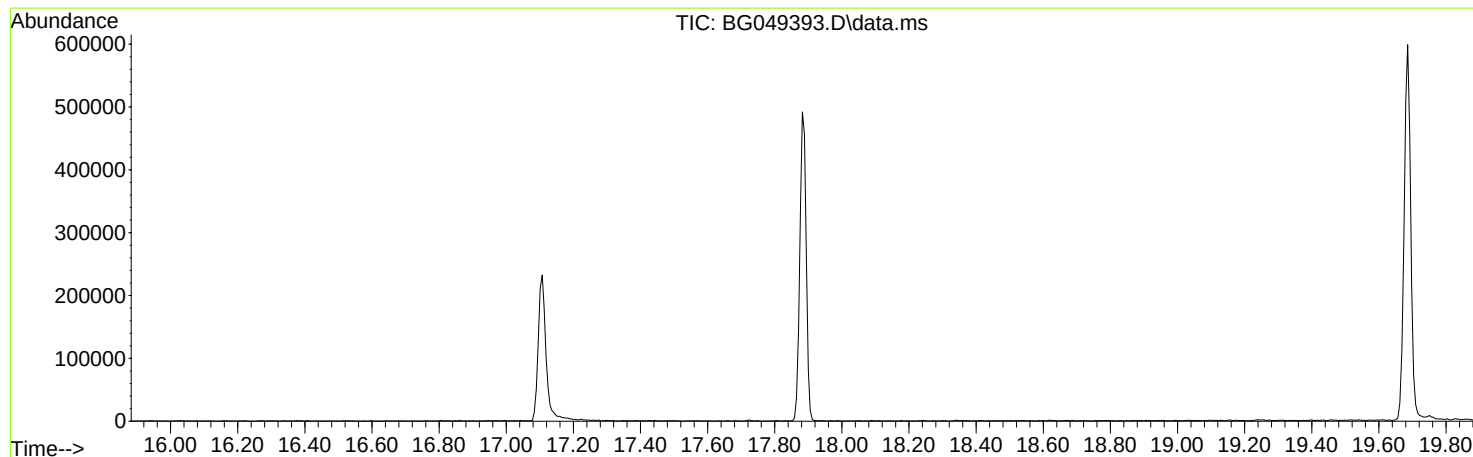

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 46.1         | 18557      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.0          | 204        | PASS                |
| 69             | 198             | 0.00            | 100             | 50.0         | 20163      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 160        | PASS                |
| 127            | 198             | 10              | 80              | 56.2         | 22624      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 40291      | PASS                |
| 199            | 198             | 5               | 9               | 6.2          | 2518       | PASS                |
| 275            | 198             | 10              | 60              | 31.5         | 12674      | PASS                |
| 365            | 198             | 1               | 100             | 5.7          | 2308       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.0         | 5621       | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 33763      | PASS                |
| 443            | 442             | 15              | 24              | 20.0         | 6765       | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/21/2021     | BNA_G            | <u>BG049393.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 136141           | 20.92              |
| DDD           | 321              | 20.47              |
| DDE           | 157              | 19.99              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 478           | 136619           | 0.35               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072121\  
Data File : BG049393.D  
Acq On : 21 Jul 2021 10:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jul 21 12:53:38 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG072121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 21 11:36:30 2021  
Response via : Initial Calibration

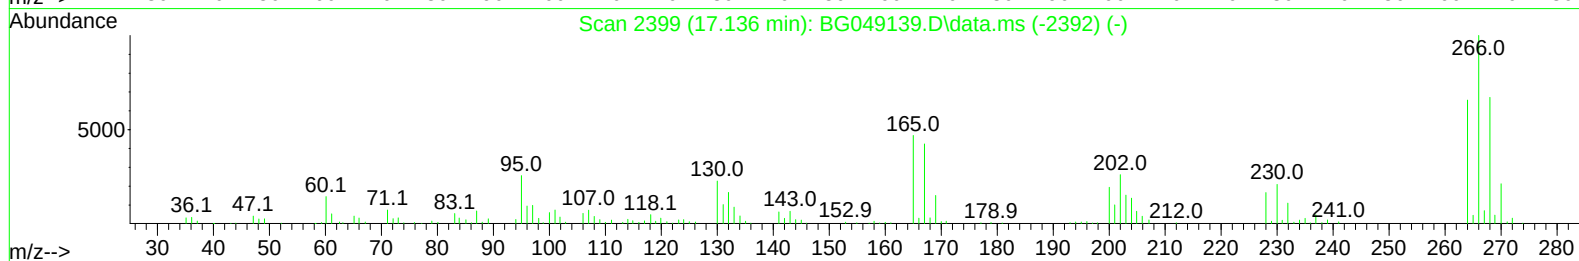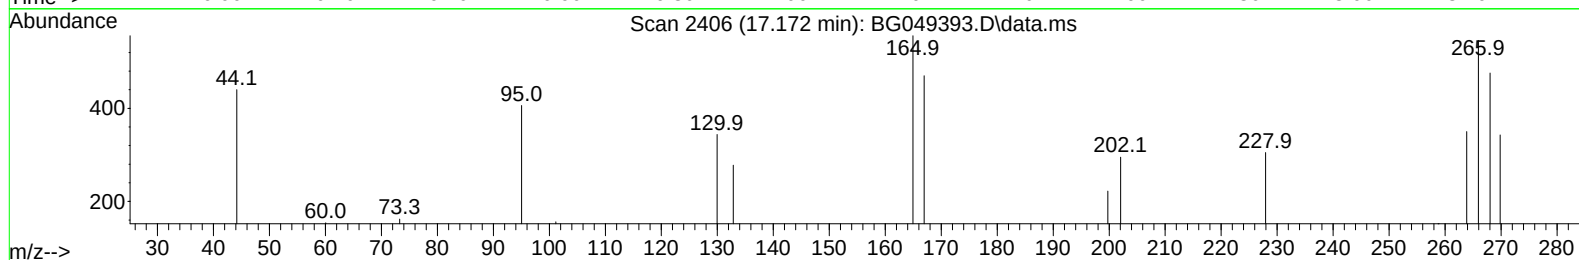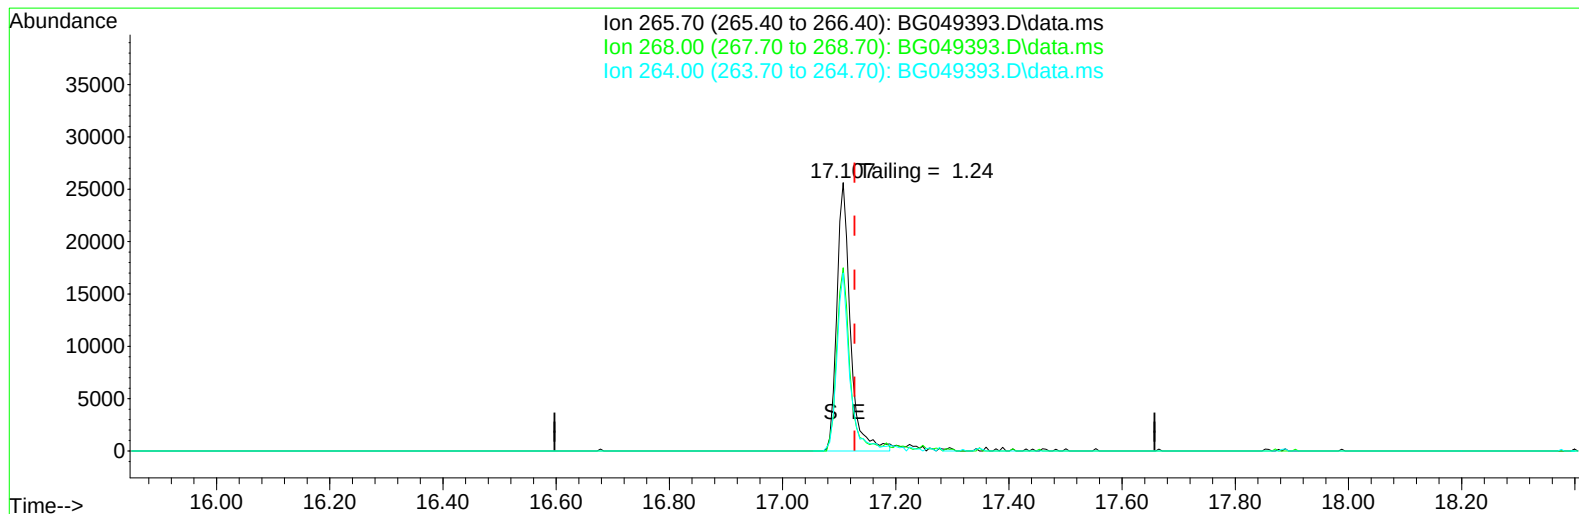

TIC: BG049393.D\data.ms

**(70) Pentachlorophenol (C)**

17.107min (-0.020) 22426.16 ng




response 41859

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 68.26  |
| 264.00 | 61.30  | 66.35  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072121\  
Data File : BG049393.D  
Acq On : 21 Jul 2021 10:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jul 21 12:53:38 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG072121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 21 11:36:30 2021  
Response via : Initial Calibration

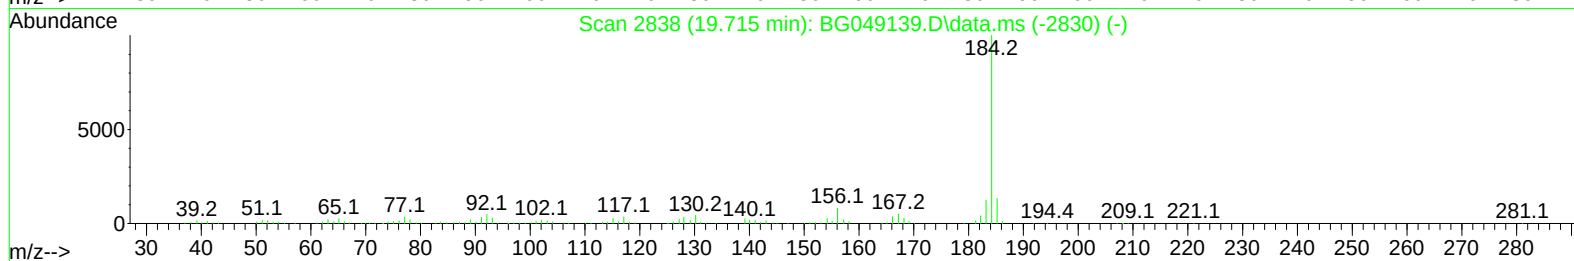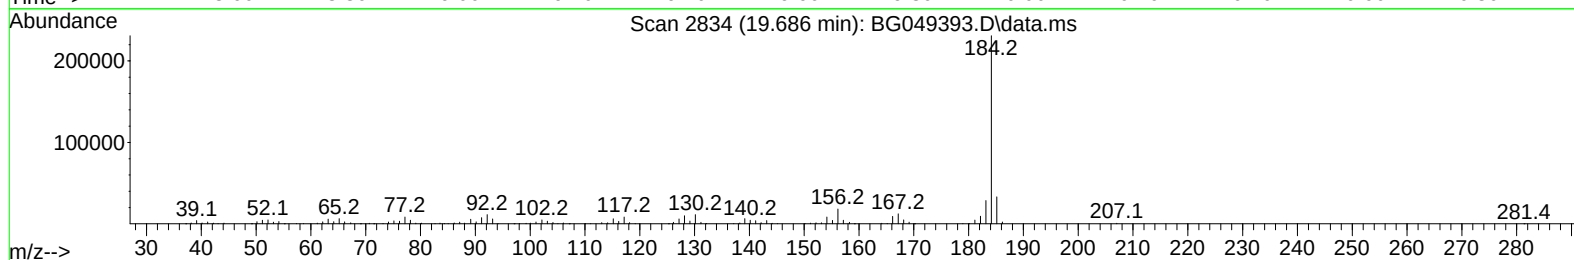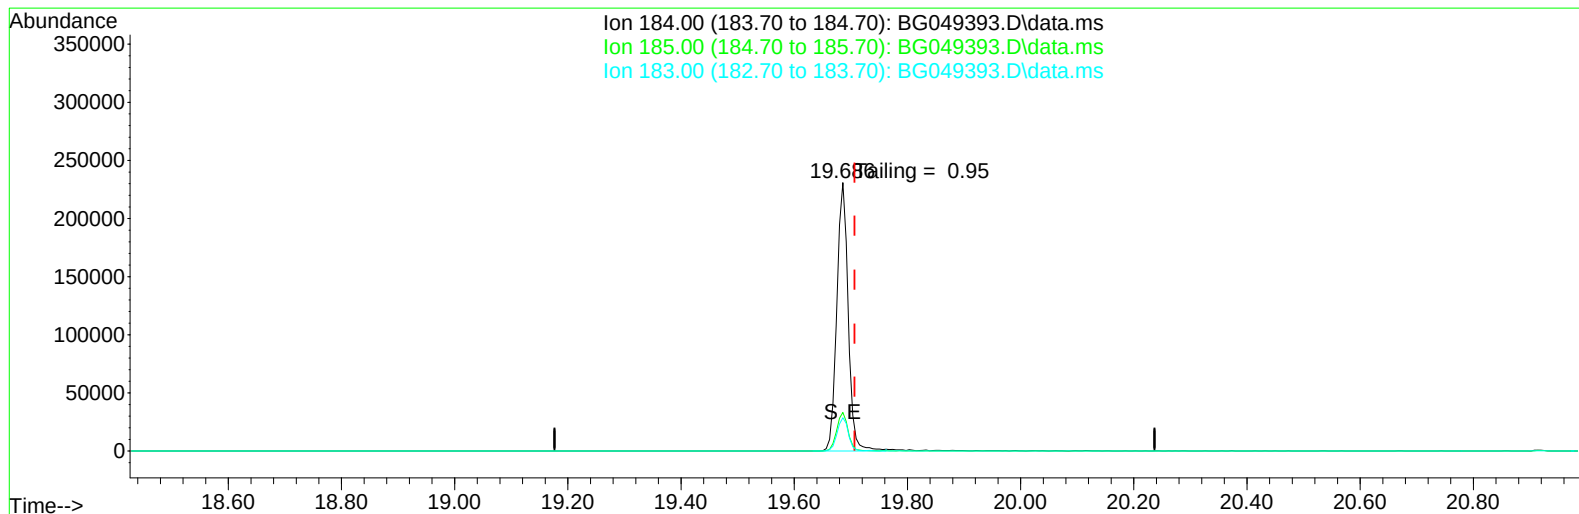

TIC: BG049393.D\data.ms

**(77) Benzidine**

19.686min (-0.020) 0.00 ng

response 321978

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 14.38  |
| 183.00 | 11.70  | 12.41  |
| 0.00   | 0.00   | 0.00   |