

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
 Data File : BG054343.D
 Acq On : 21 Jul 2022 13:29
 Operator : CG/JU
 Sample : N3771-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-10F

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.573	366	372	382	rVB	148606	251843	11.13%	1.616%
2	7.177	637	645	653	rBV2	92880	167184	7.39%	1.073%
3	8.000	777	785	791	rBV	71627	123324	5.45%	0.792%
4	8.059	791	795	805	rVB	23064	41295	1.83%	0.265%
5	8.822	919	925	933	rVB	17570	30254	1.34%	0.194%
6	9.104	966	973	977	rBV	34964	59281	2.62%	0.380%
7	9.163	977	983	994	rVB	234527	433234	19.15%	2.781%
8	10.573	1217	1223	1233	rBV	40392	72353	3.20%	0.464%
9	10.808	1256	1263	1270	rBV2	87626	162334	7.18%	1.042%
10	11.161	1315	1323	1333	rBV	62563	120523	5.33%	0.774%
11	11.337	1345	1353	1358	rBV	308578	537079	23.74%	3.447%
12	11.402	1358	1364	1379	rVB	397896	683753	30.23%	4.389%
13	11.666	1404	1409	1417	rVB2	14996	27387	1.21%	0.176%
14	13.252	1671	1679	1687	rVB	714719	1143269	50.54%	7.338%
15	14.633	1907	1914	1923	rVB	153982	255120	11.28%	1.637%
16	16.126	2161	2168	2179	rBV2	690723	1098237	48.55%	7.049%
17	16.772	2273	2278	2284	rBV3	22783	34055	1.51%	0.219%
18	17.377	2375	2381	2387	rVB	208002	321087	14.19%	2.061%
19	17.553	2400	2411	2413	rBV8	16362	44857	1.98%	0.288%
20	18.270	2527	2533	2541	rBV	282581	426913	18.87%	2.740%
21	18.341	2542	2545	2549	rVB3	17258	25683	1.14%	0.165%
22	18.999	2653	2657	2663	rBV	17946	26521	1.17%	0.170%
23	19.416	2720	2728	2737	rBV4	49121	147757	6.53%	0.948%
24	19.539	2744	2749	2758	rBV	361738	547852	24.22%	3.516%
25	19.950	2809	2819	2820	rBV	72610	147799	6.53%	0.949%
26	19.992	2820	2826	2834	rVB	1496828	2102835	92.96%	13.497%
27	20.526	2913	2917	2921	rVB	27946	39262	1.74%	0.252%
28	21.184	3023	3029	3039	rVB2	78880	225152	9.95%	1.445%
29	21.284	3043	3046	3054	rVV5	21254	39244	1.73%	0.252%
30	21.408	3061	3067	3079	rBV4	51998	145585	6.44%	0.934%
31	21.648	3102	3108	3114	rVB	240538	419439	18.54%	2.692%
32	21.954	3157	3160	3169	rVB3	26532	46890	2.07%	0.301%
33	22.518	3251	3256	3264	rVB5	49069	135075	5.97%	0.867%
34	23.106	3348	3356	3368	rVB2	256990	545066	24.10%	3.499%
35	23.311	3388	3391	3397	rVB2	19305	34227	1.51%	0.220%
36	24.386	3566	3574	3578	rBV6	41007	121326	5.36%	0.779%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054343.D
Acq On : 21 Jul 2022 13:29
Operator : CG/JU
Sample : N3771-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10F

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	24.851	3641	3653	3666	rVB3	793126	2262058	100.00%	14.519%
38	27.324	4060	4074	4088	rVB2	374522	1475785	65.24%	9.472%
39	30.902	4670	4683	4704	rVB6	185060	1059006	46.82%	6.797%




Sum of corrected areas: 15579944

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054343.D
Acq On : 21 Jul 2022 13:29
Operator : CG/JU
Sample : N3771-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

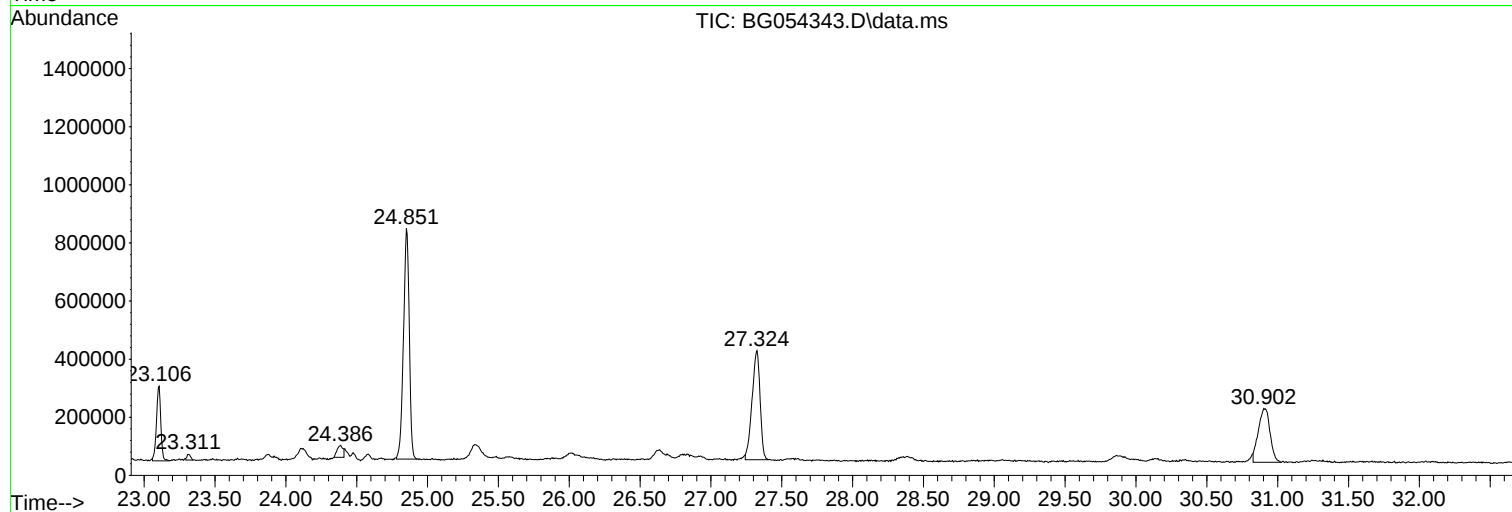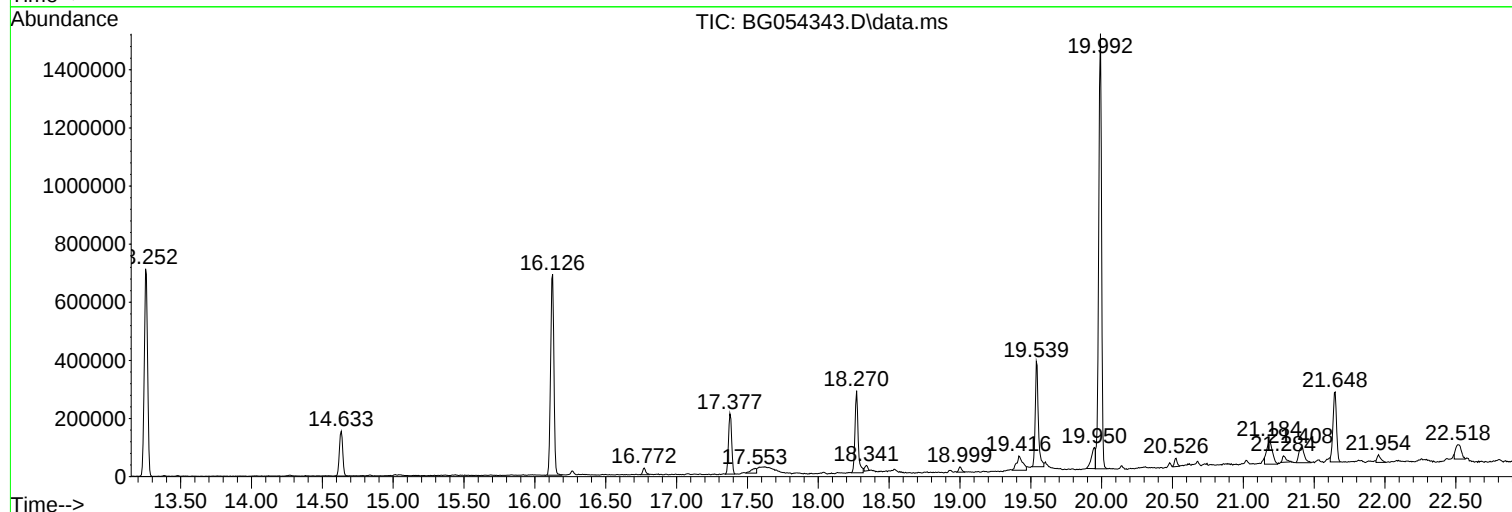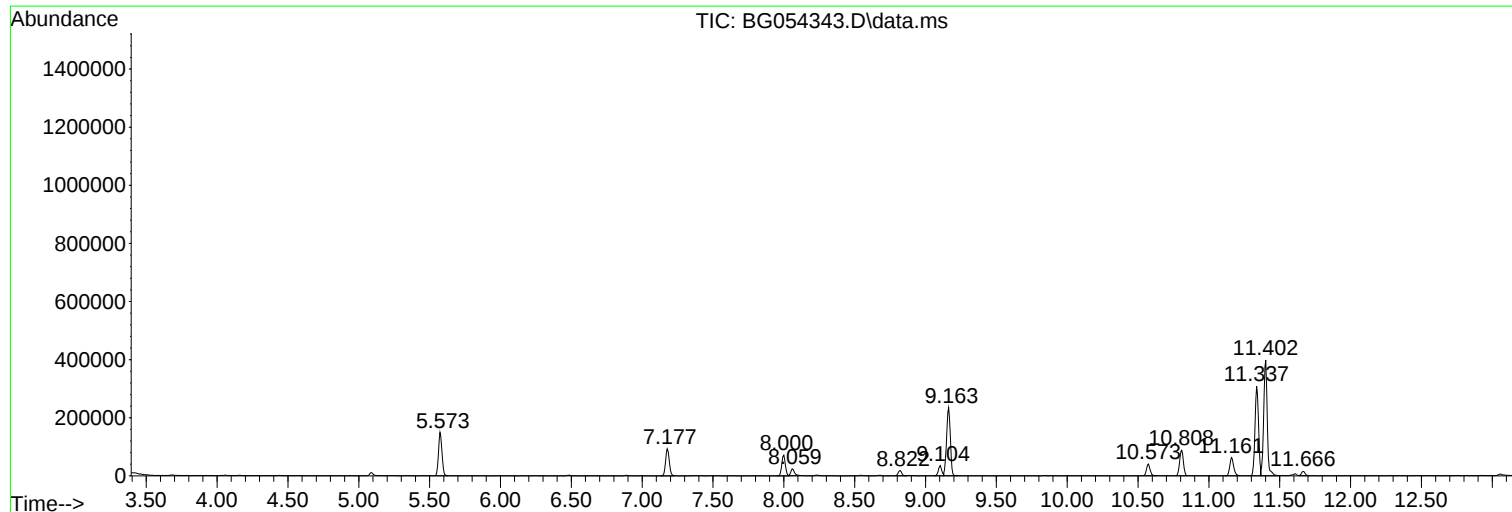

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054343.D
Acq On : 21 Jul 2022 13:29
Operator : CG/JU
Sample : N3771-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054343.D
Acq On : 21 Jul 2022 13:29
Operator : CG/JU
Sample : N3771-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc