

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
 Data File : BG054346.D
 Acq On : 21 Jul 2022 15:37
 Operator : CG/JU
 Sample : N3786-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 0718-WC-TP-WC3EB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.573	365	372	382	rVB	143904	250358	26.30%	5.236%
2	7.177	638	645	654	rBV	154530	277285	29.13%	5.799%
3	7.994	778	784	791	rVB	66560	113690	11.94%	2.378%
4	9.157	974	982	994	rBB	96484	177317	18.63%	3.709%
5	10.808	1255	1263	1272	rBV	82950	156909	16.48%	3.282%
6	13.253	1672	1679	1687	rBB	305987	473670	49.76%	9.907%
7	14.633	1907	1914	1921	rBB	160787	255900	26.88%	5.352%
8	16.120	2161	2167	2178	rBV3	330990	514598	54.06%	10.763%
9	17.377	2372	2381	2386	rBV	244260	369297	38.80%	7.724%
10	17.507	2396	2403	2408	rBV	10712	16609	1.74%	0.347%
11	18.264	2527	2532	2536	rBV3	13914	21546	2.26%	0.451%
12	19.428	2723	2730	2735	rBV	48967	70783	7.44%	1.480%
13	19.763	2782	2787	2788	rBV2	11831	16022	1.68%	0.335%
14	19.792	2788	2792	2798	rVB	41644	66566	6.99%	1.392%
15	19.986	2819	2825	2831	rBV	731226	951860	100.00%	19.908%
16	20.115	2841	2847	2849	rBV7	8341	16633	1.75%	0.348%
17	20.250	2866	2870	2874	rBV6	5603	11855	1.25%	0.248%
18	21.284	3041	3046	3051	rBV3	20712	32720	3.44%	0.684%
19	21.643	3100	3107	3113	rBV	280699	496512	52.16%	10.385%
20	21.690	3113	3115	3119	rVB	18681	21911	2.30%	0.458%
21	24.851	3643	3653	3664	rBV2	162442	469161	49.29%	9.813%




Sum of corrected areas: 4781202

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054346.D
Acq On : 21 Jul 2022 15:37
Operator : CG/JU
Sample : N3786-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0718-WC-TP-WC3EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

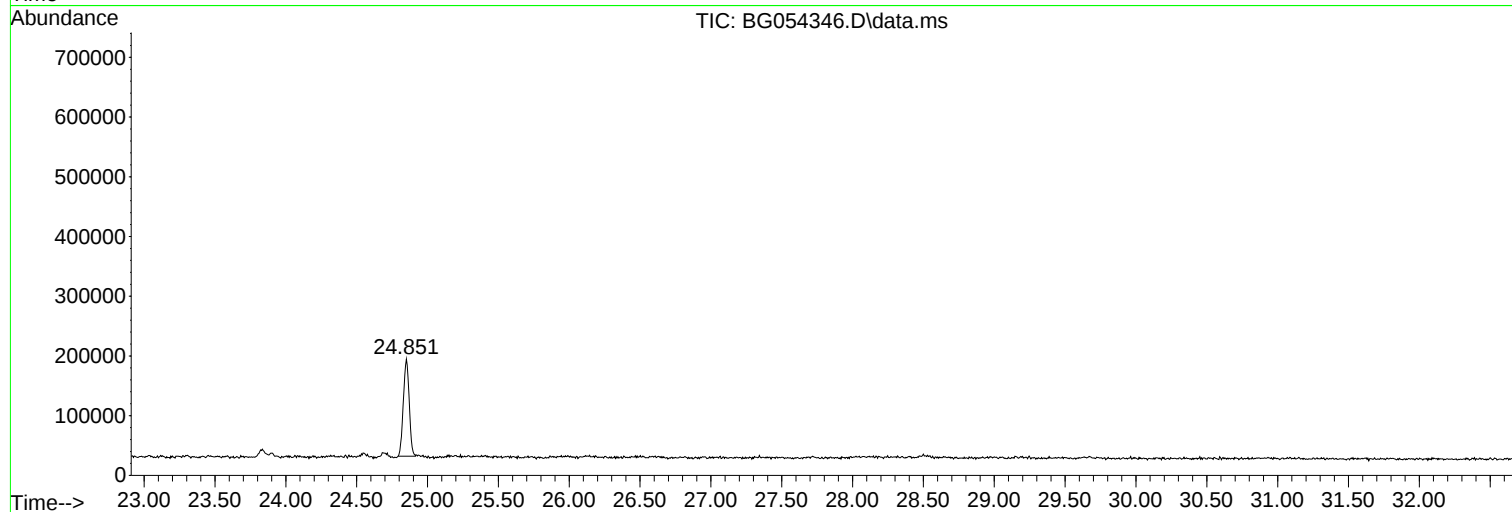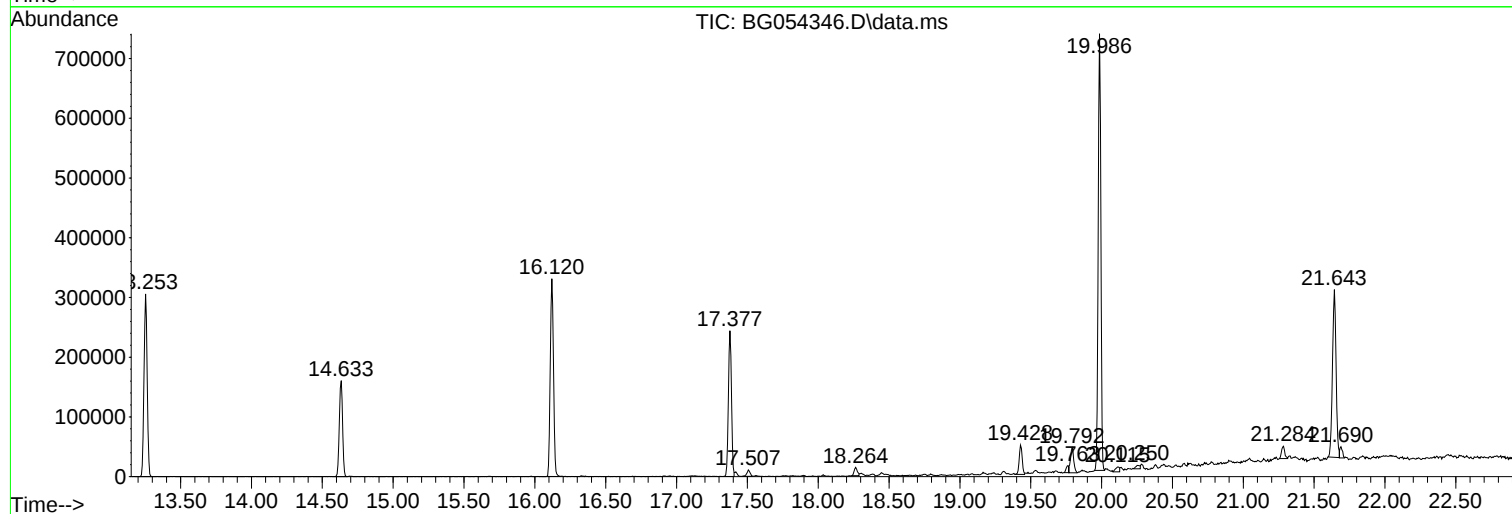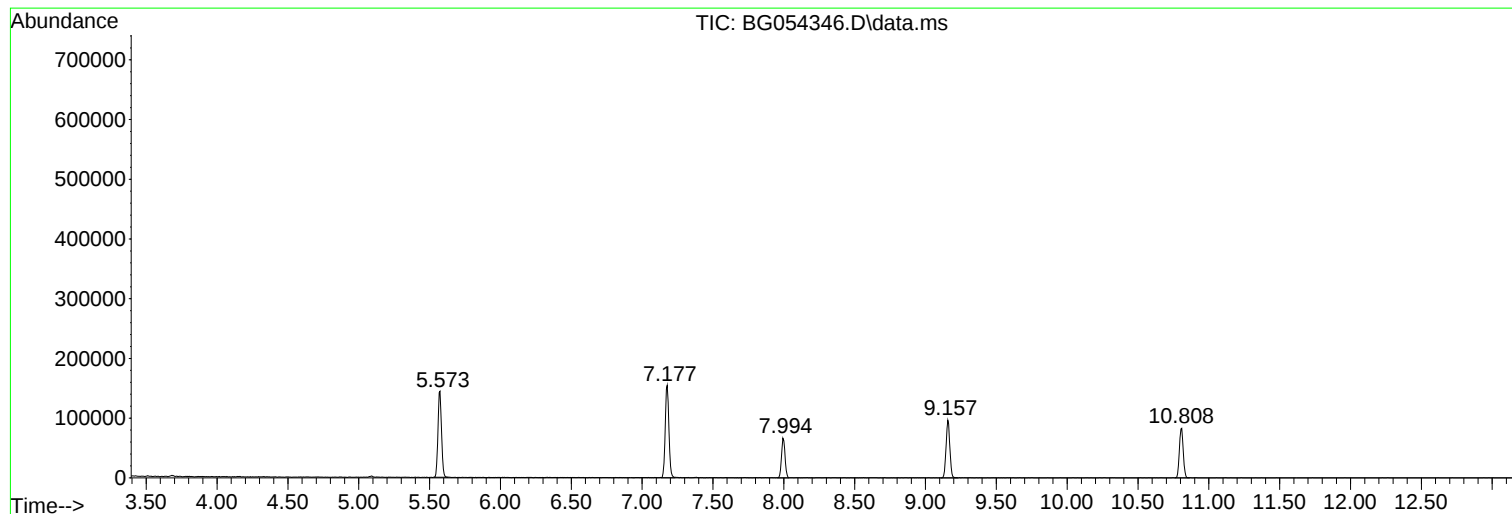

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054346.D
Acq On : 21 Jul 2022 15:37
Operator : CG/JU
Sample : N3786-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0718-WC-TP-WC3EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072122\
Data File : BG054346.D
Acq On : 21 Jul 2022 15:37
Operator : CG/JU
Sample : N3786-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
0718-WC-TP-WC3EB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------