
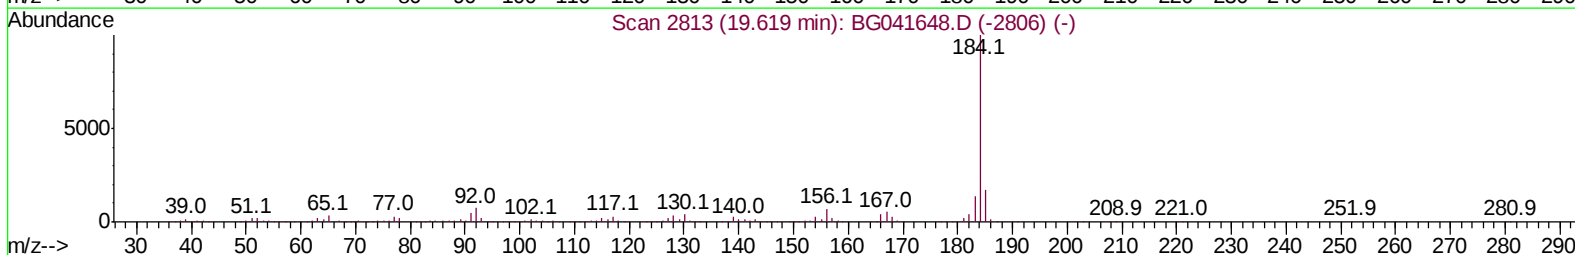
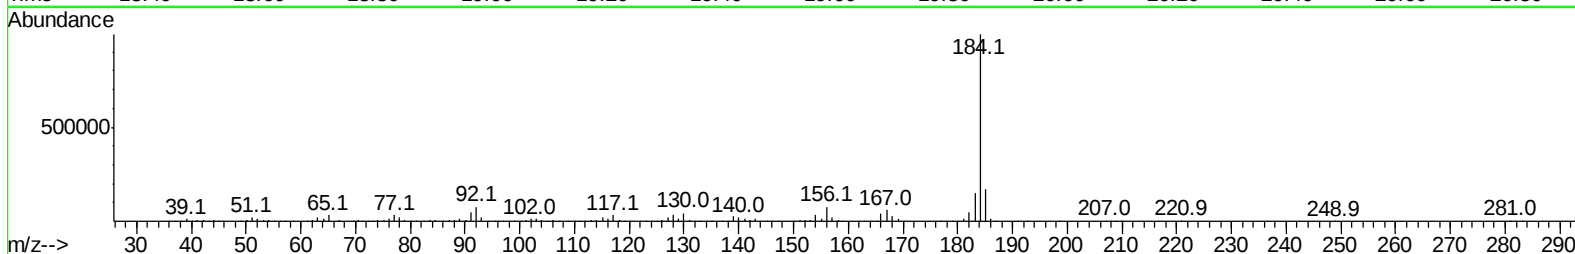


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072219\
 Data File : BG041741.D
 Acq On : 22 Jul 2019 9:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:40:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 15 16:16:21 2019
 Response via : Initial Calibration

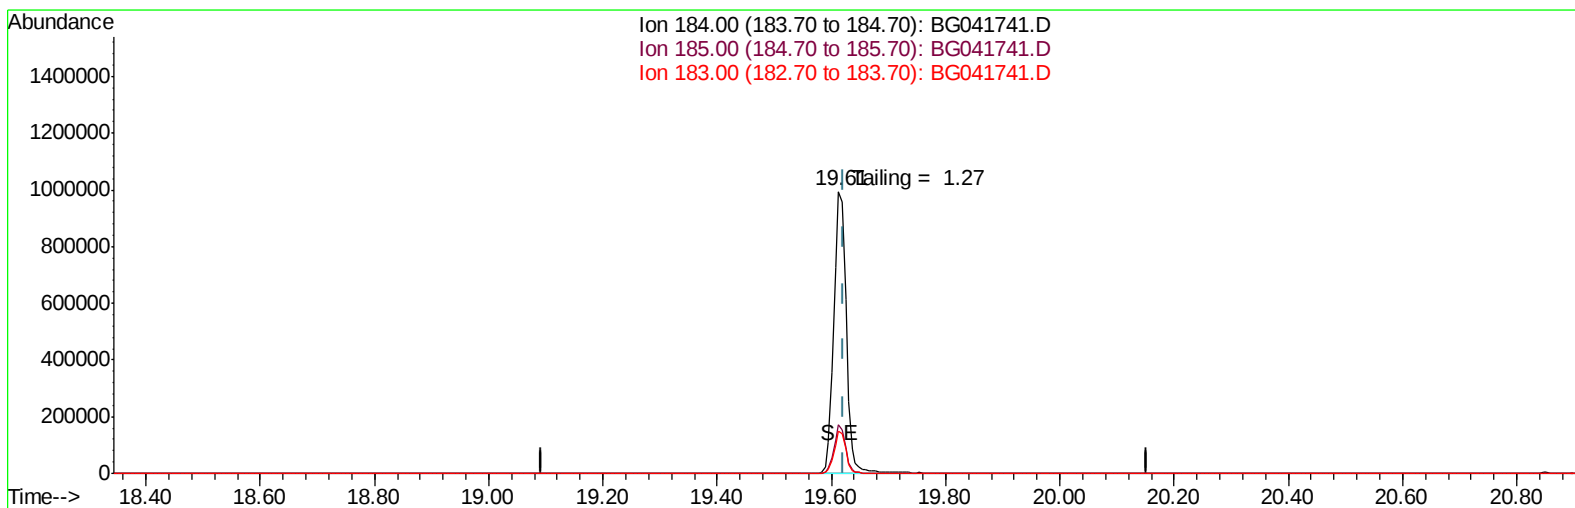

TIC: BG041741.D

(77) Benzidine




19.613min (-0.010) -20.00ng

response 1508503

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	17.09
183.00	14.70	14.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072219\
Data File : BG041741.D
Acq On : 22 Jul 2019 9:36
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:40:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

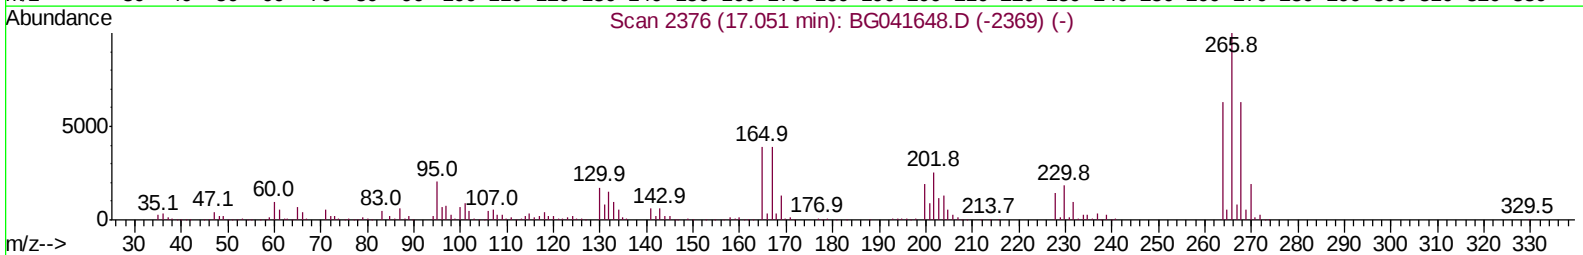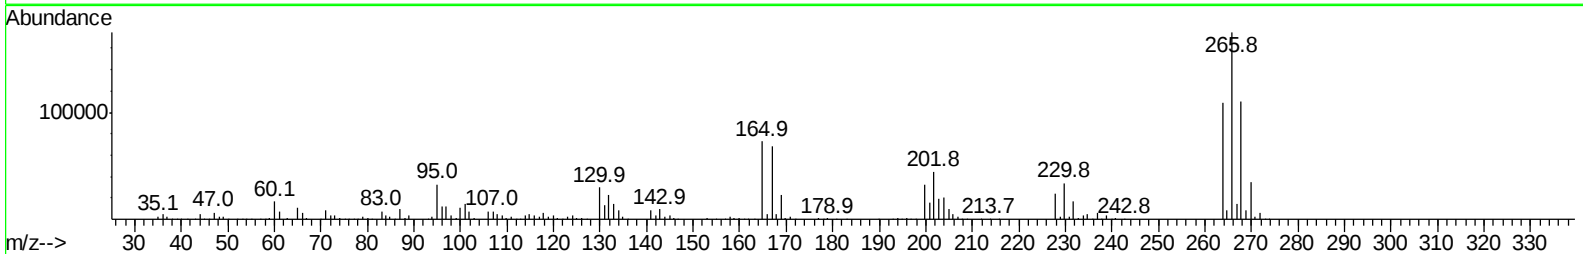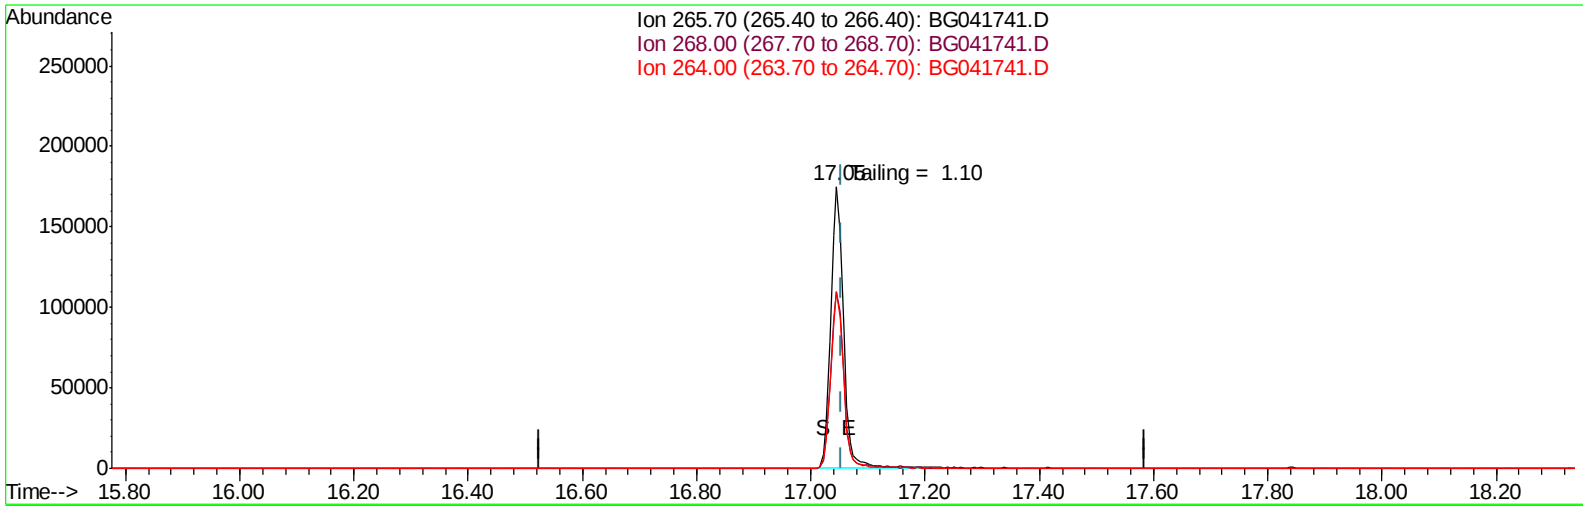

TIC: BG041741.D

(70) Pentachlorophenol (C)

17.045min (-0.010) 111054.16ng

response 268735

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	62.88
264.00	64.30	62.69
0.00	0.00	0.00