


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072219\
 Data File : BG041741.D
 Acq On : 22 Jul 2019 9:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

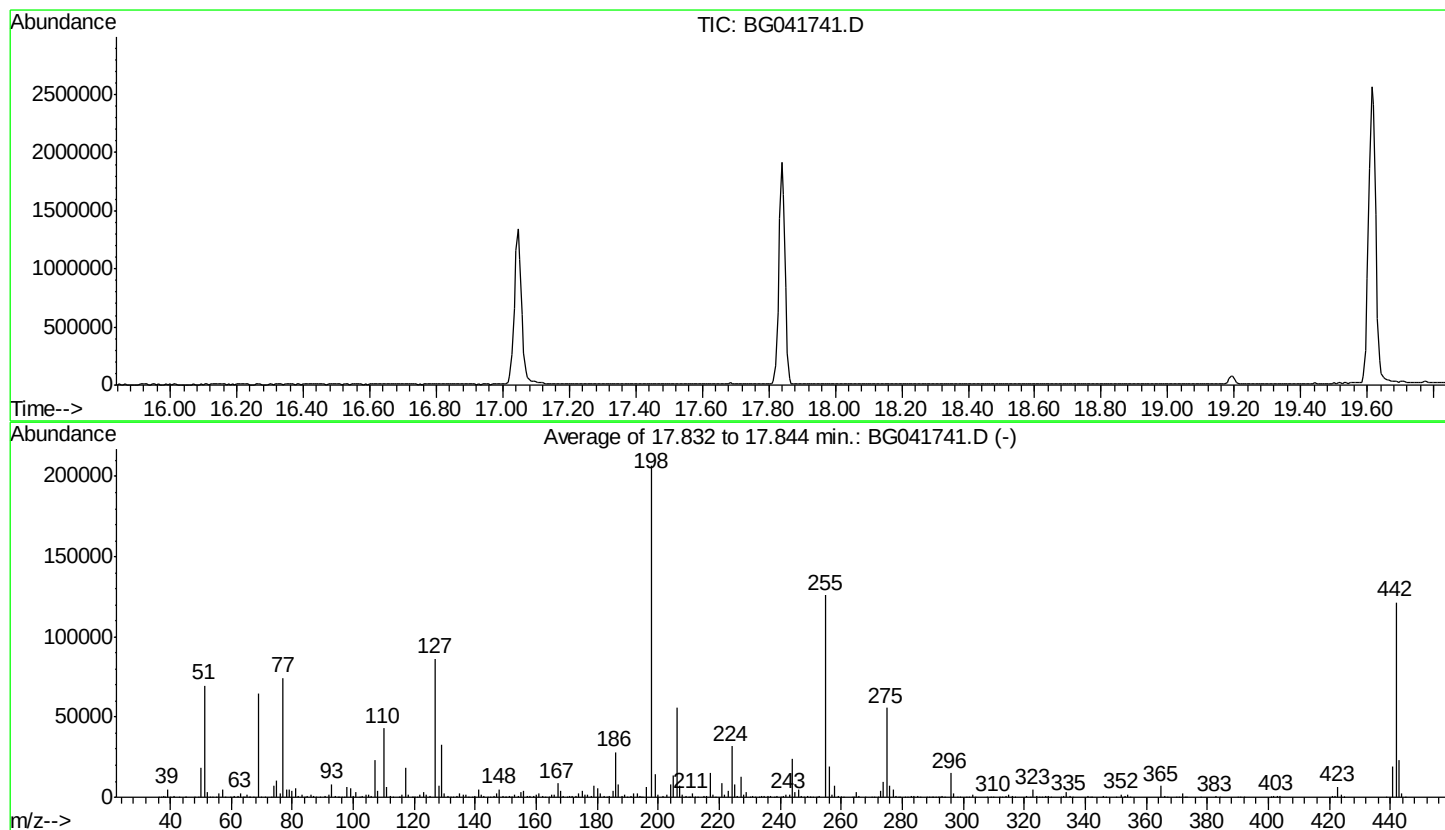

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	69504	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	65026	PASS
70	69	0.00	2	0.4	273	PASS
127	198	10	80	41.8	86504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	206784	PASS
199	198	5	9	6.8	14116	PASS
275	198	10	60	26.9	55608	PASS
365	198	1	100	3.3	6877	PASS
441	198	0.01	100	9.4	19362	PASS
442	198	50	100	58.9	121754	PASS
443	442	15	24	19.2	23429	PASS