
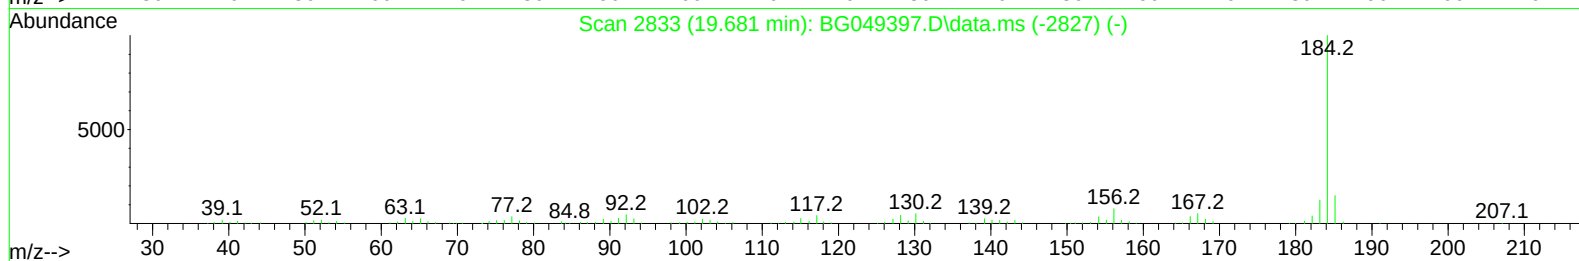
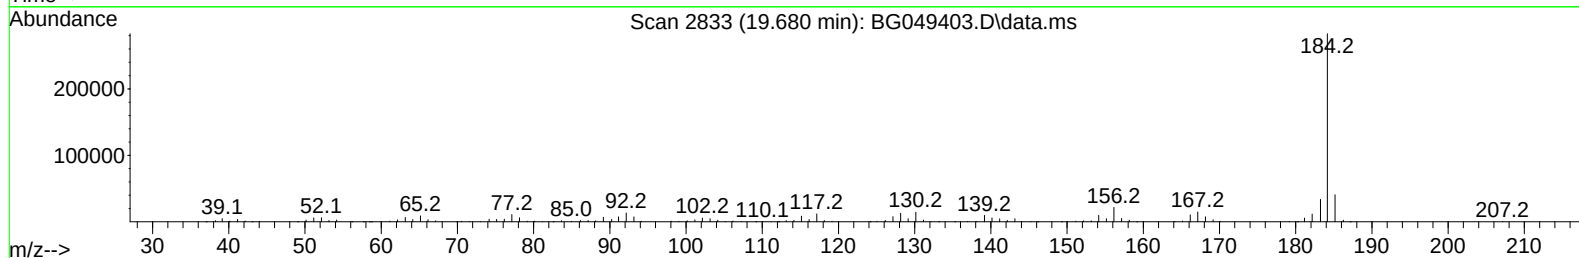


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049403.D
Acq On : 22 Jul 2021 7:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 10:49:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

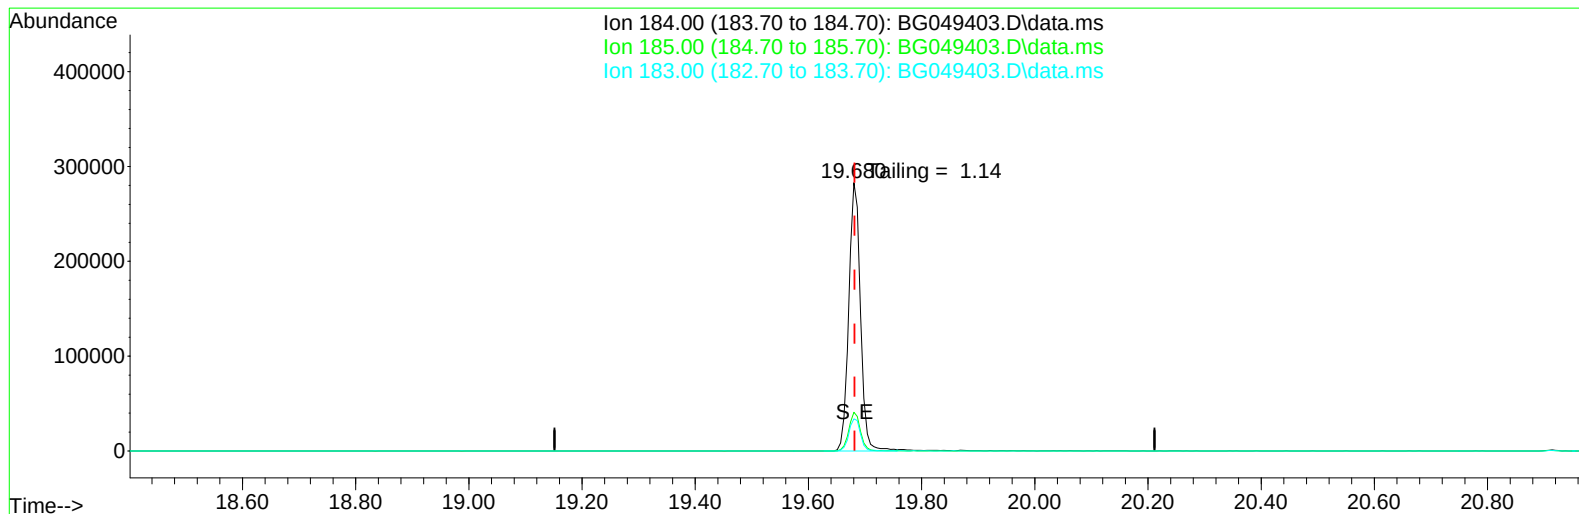

TIC: BG049403.D\data.ms

(77) Benzidine




19.680min (-0.001) 0.00 ng

response 407619

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.45
183.00	11.70	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049403.D
Acq On : 22 Jul 2021 7:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 10:49:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

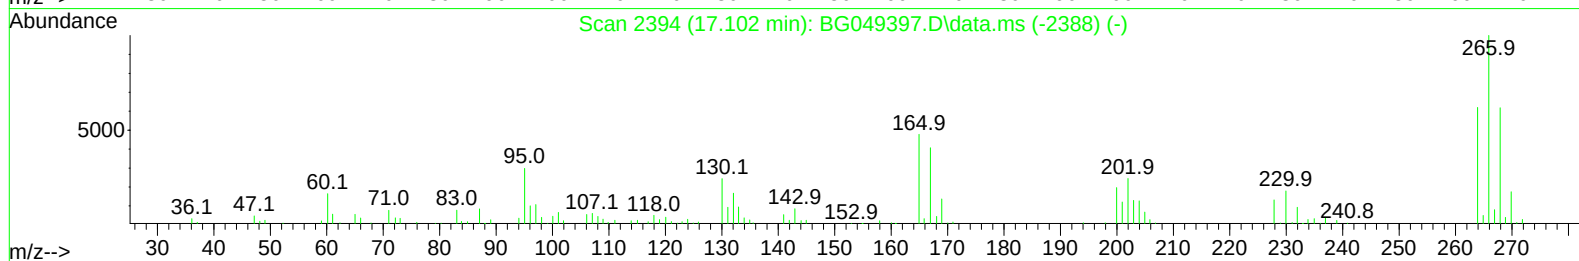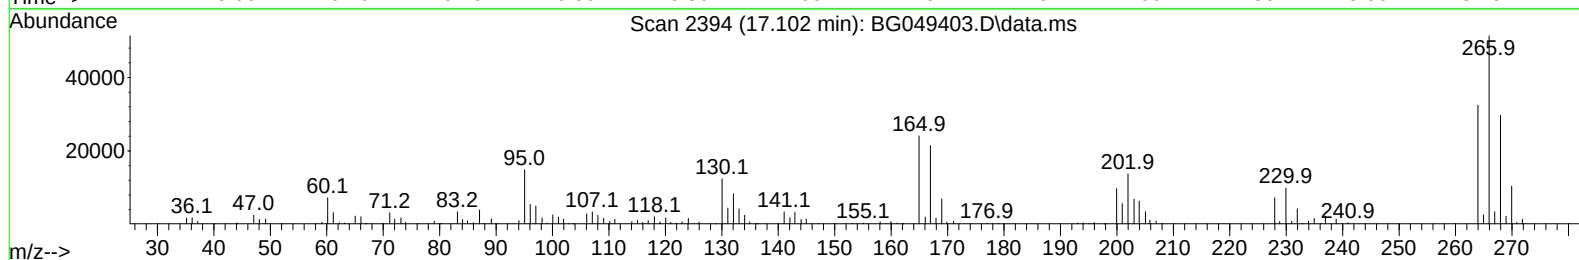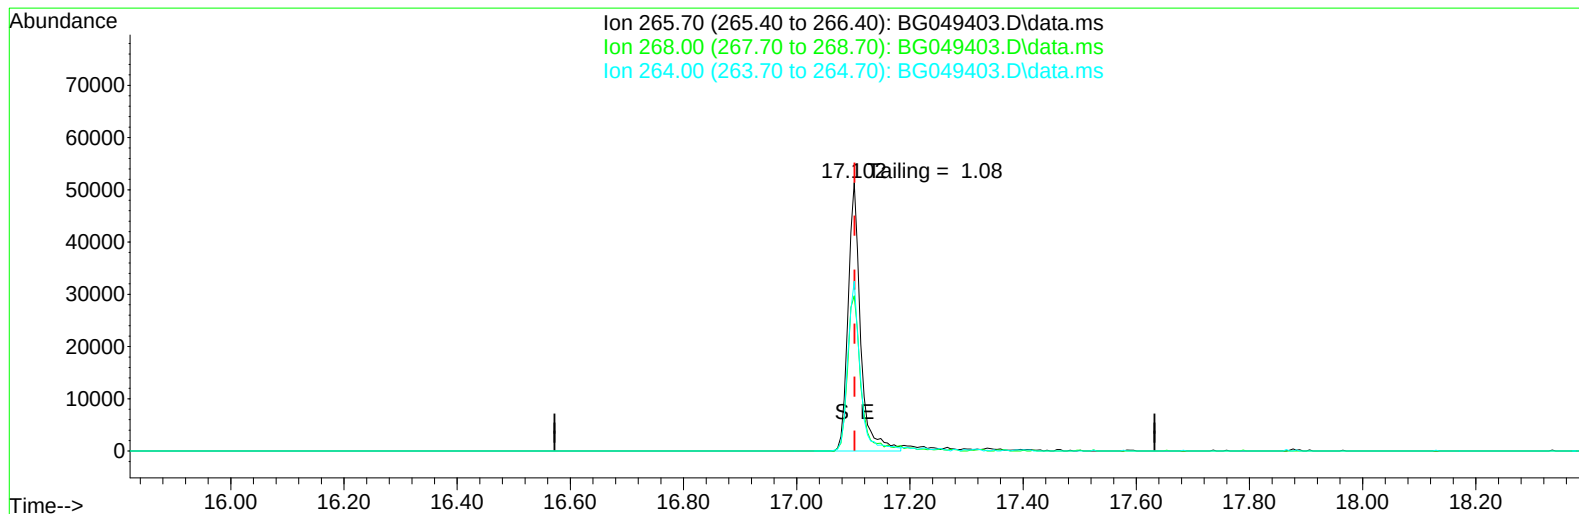

TIC: BG049403.D\data.ms

(70) Pentachlorophenol (C)

17.102min (-0.000) 30467.23 ng

response 78407

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	57.83
264.00	61.30	63.19
0.00	0.00	0.00