
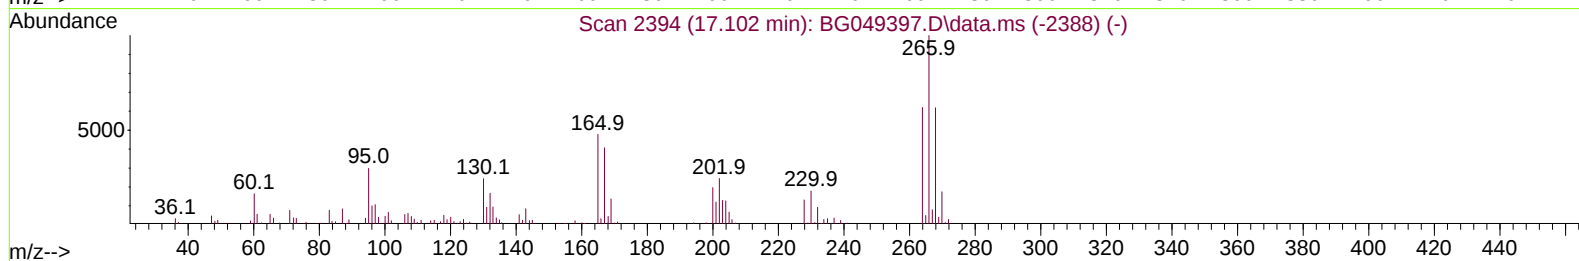
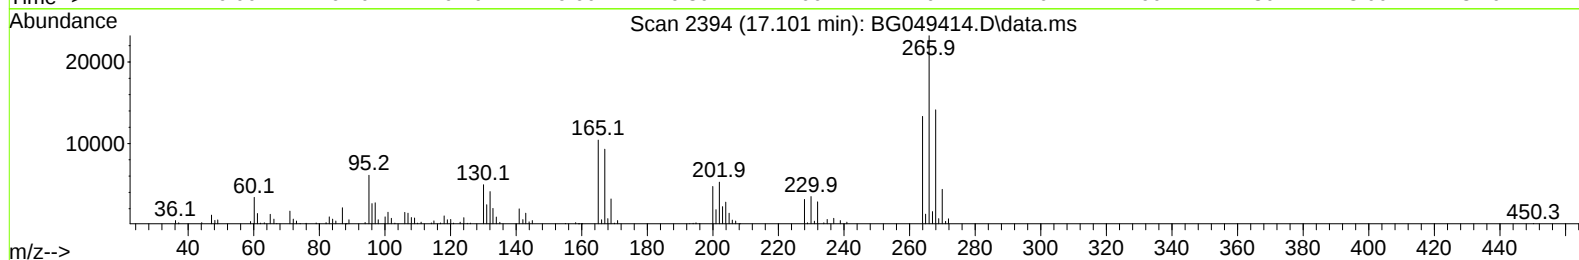


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049414.D
Acq On : 22 Jul 2021 20:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 03:27:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

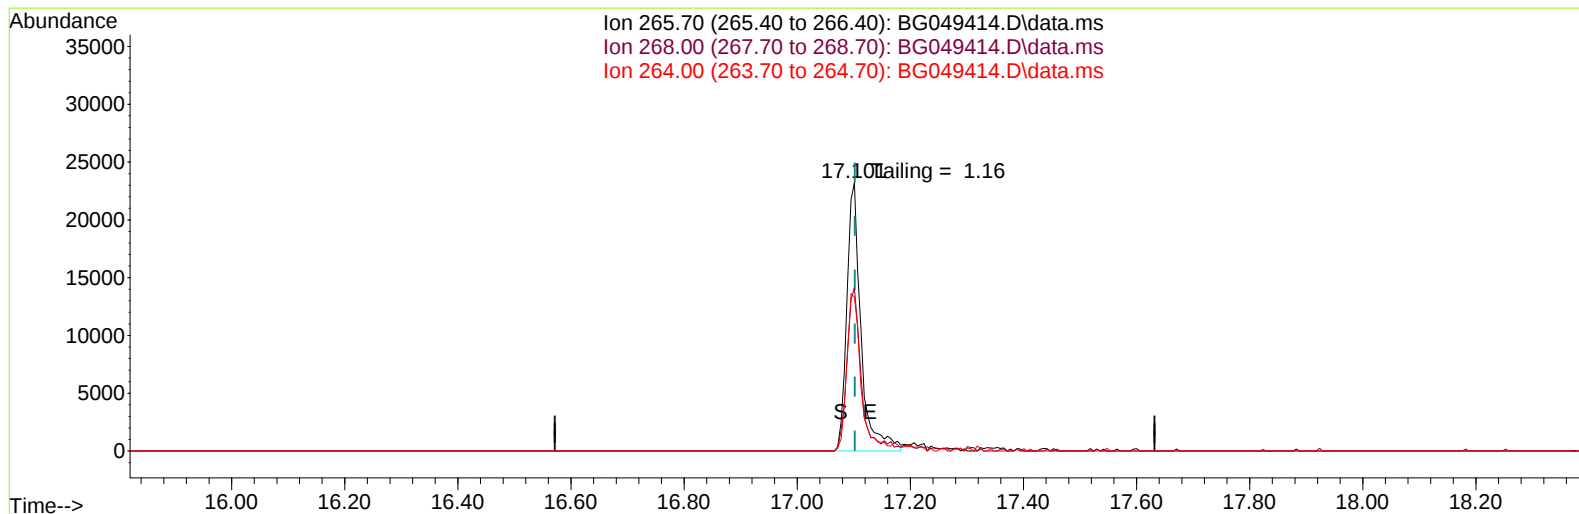

TIC: BG049414.D\data.ms

(70) Pentachlorophenol (C)




17.101min (-0.001) 23156.67 ng

response 41108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.83
264.00	61.30	57.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049414.D
Acq On : 22 Jul 2021 20:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 03:27:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

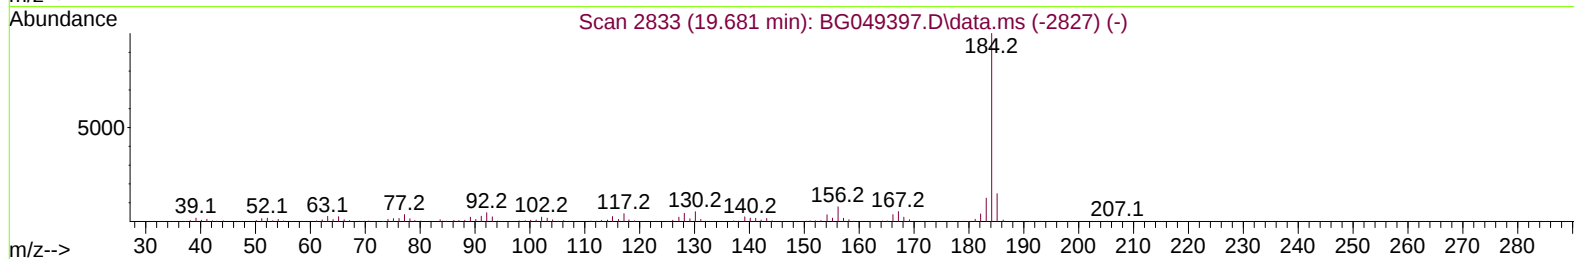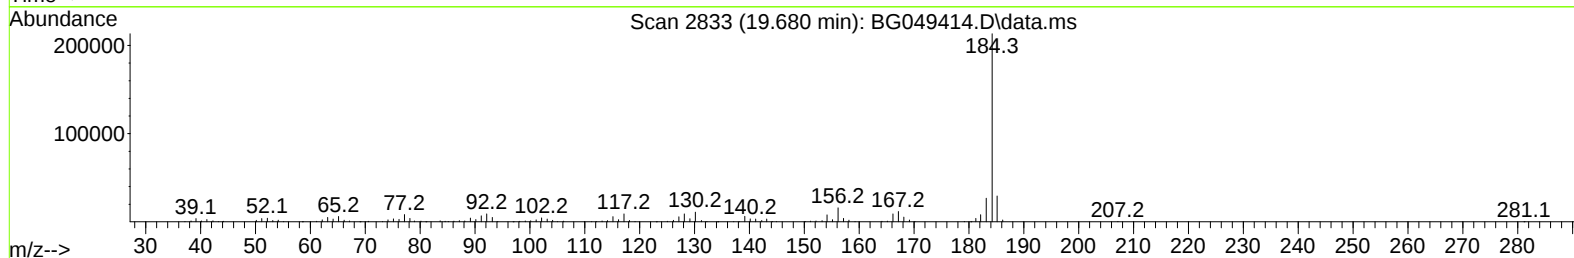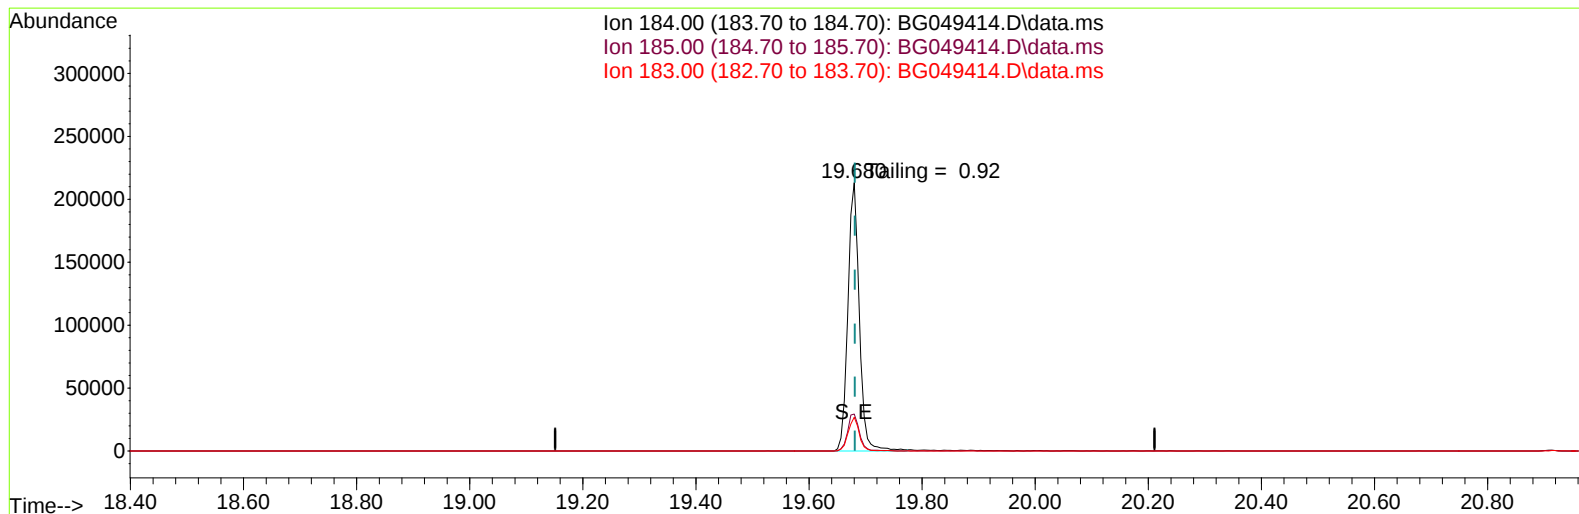

TIC: BG049414.D\data.ms

(77) Benzidine**19.680min (-0.001) 193350.51 ng****response 299675**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.77
183.00	11.70	12.58
0.00	0.00	0.00