
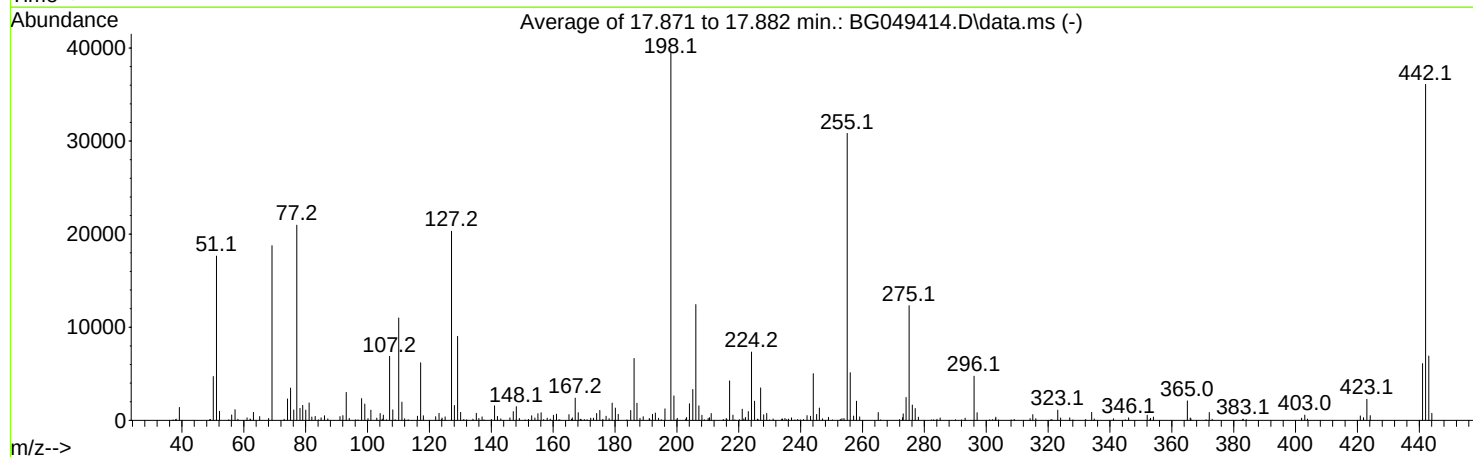


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
 Data File : BG049414.D
 Acq On : 22 Jul 2021 20:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 16:57:05 2021

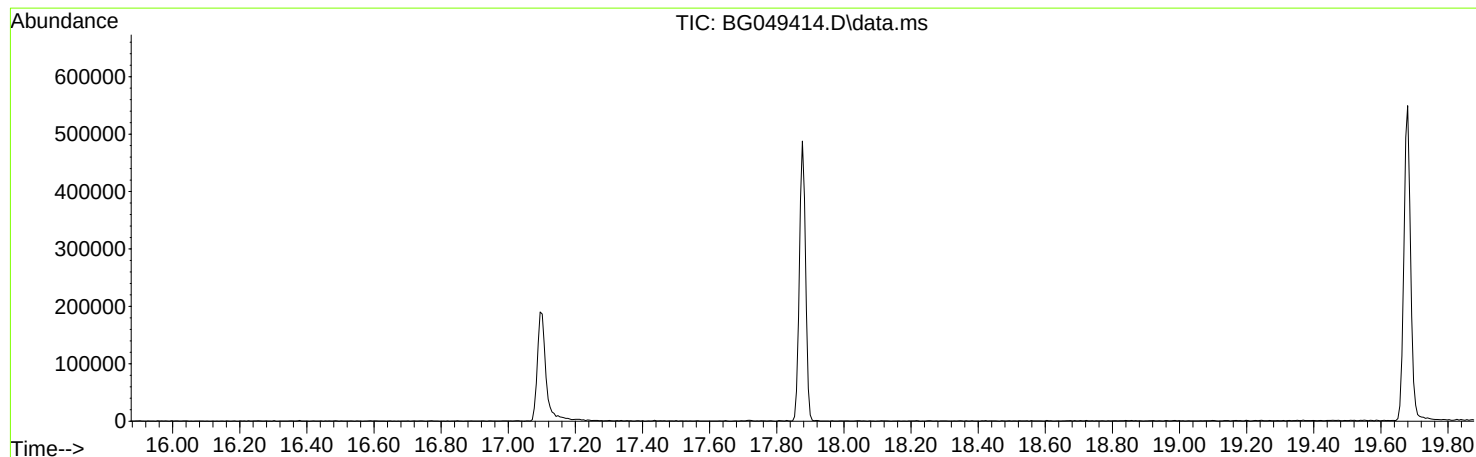




AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	17659	PASS
68	69	0.00	2	1.1	204	PASS
69	198	0.00	100	47.5	18760	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	20320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39512	PASS
199	198	5	9	6.7	2638	PASS
275	198	10	60	31.2	12325	PASS
365	198	1	100	5.3	2099	PASS
441	198	0.01	100	15.4	6100	PASS
442	442	100	100	100.0	36088	PASS
443	442	15	24	19.1	6903	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049414.D
Acq On : 22 Jul 2021 20:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 03:27:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

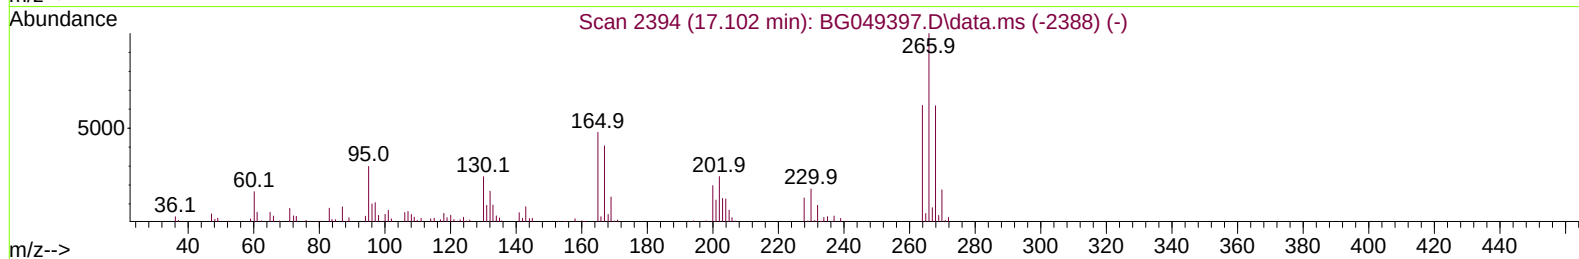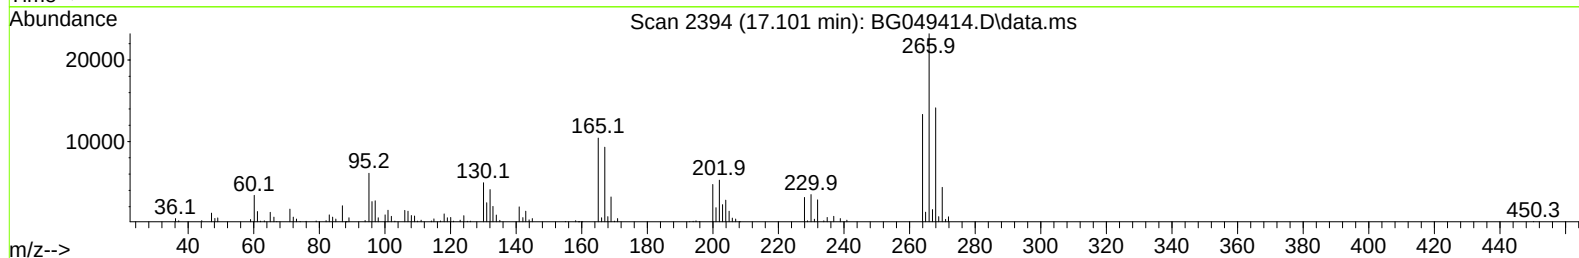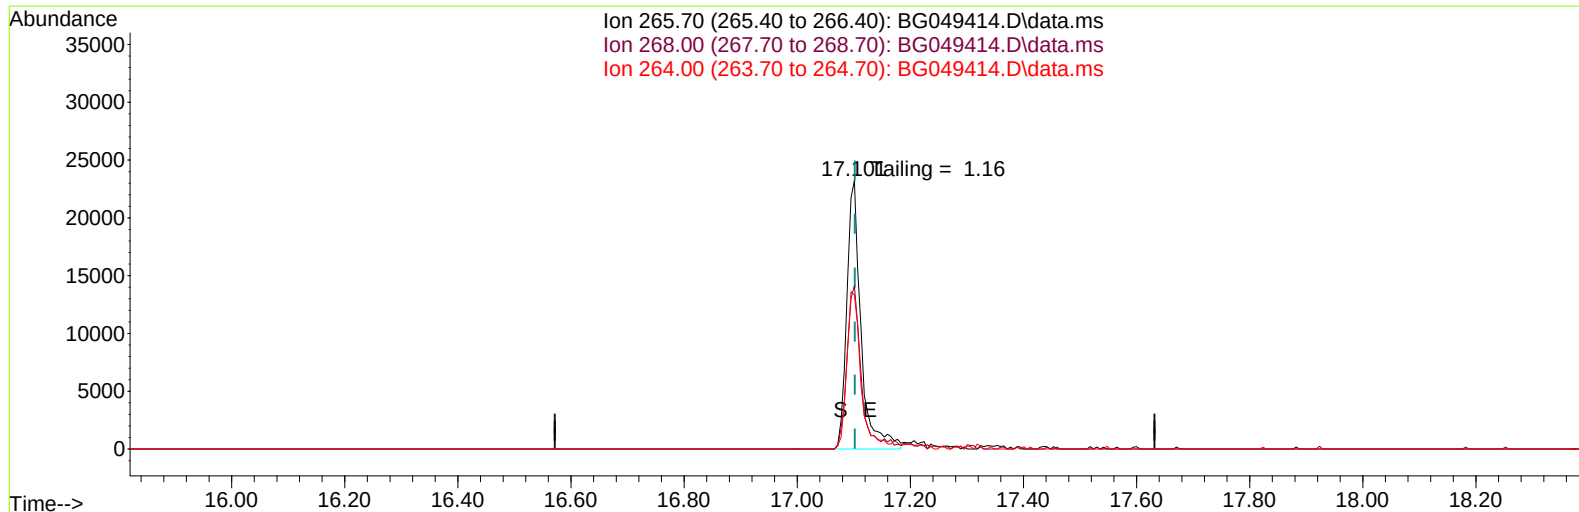

TIC: BG049414.D\data.ms

(70) Pentachlorophenol (C)

17.101min (-0.001) 23156.67 ng




response 41108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.83
264.00	61.30	57.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072221\
Data File : BG049414.D
Acq On : 22 Jul 2021 20:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 03:27:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

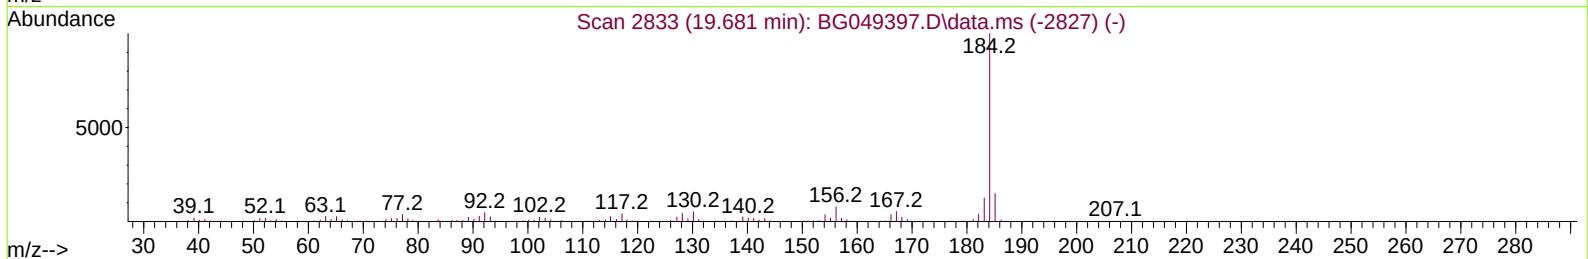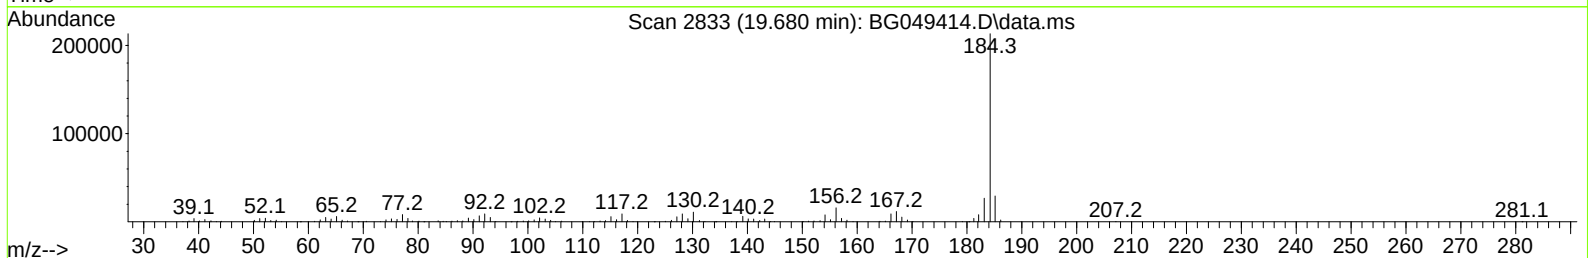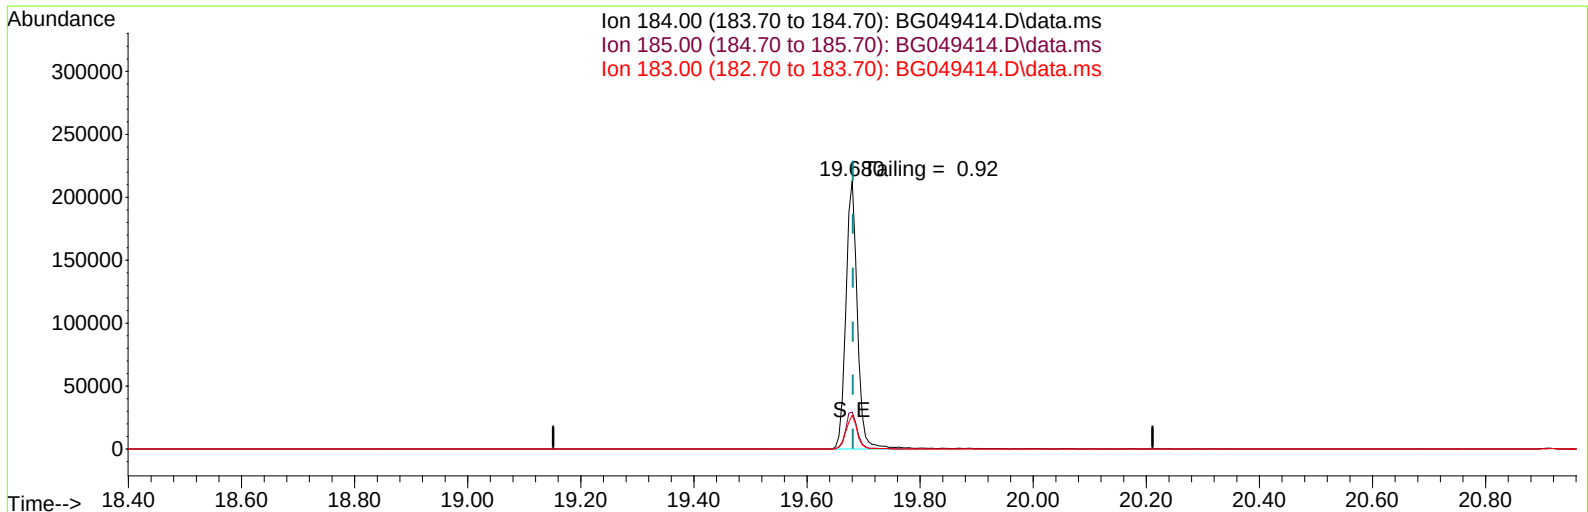

TIC: BG049414.D\data.ms

(77) Benzidine

19.680min (-0.001) 193350.51 ng

response 299675

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.77
183.00	11.70	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2021	BNA_G	<u>BG049414.D</u>
Compound Name	Response	Retention Time
DDT	148671	20.913
DDD	2333	20.467
DDE	281	19.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2614	151285	1.73

Instrument :
BNA_G
ClientSampleId :
DFTPP