
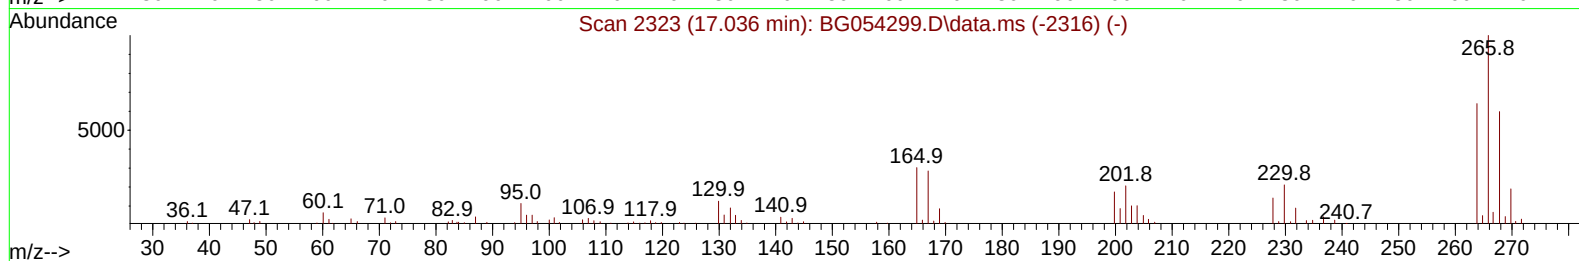
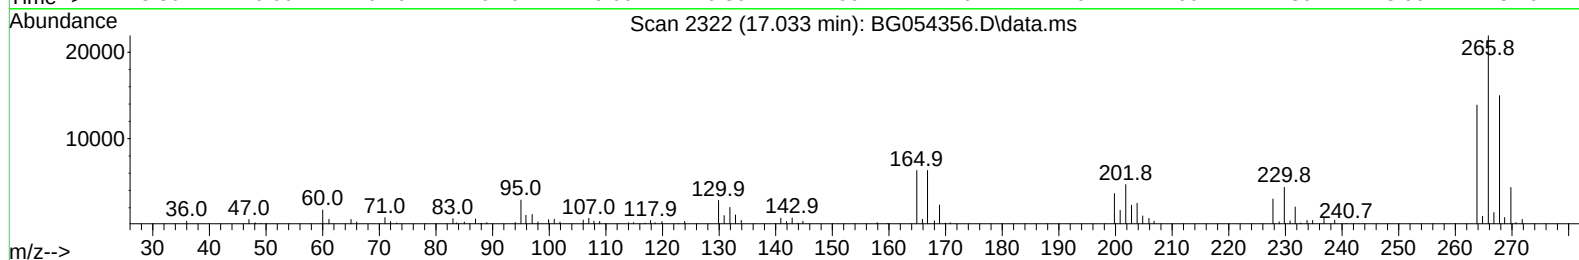


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072222\
Data File : BG054356.D
Acq On : 22 Jul 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 02:06:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

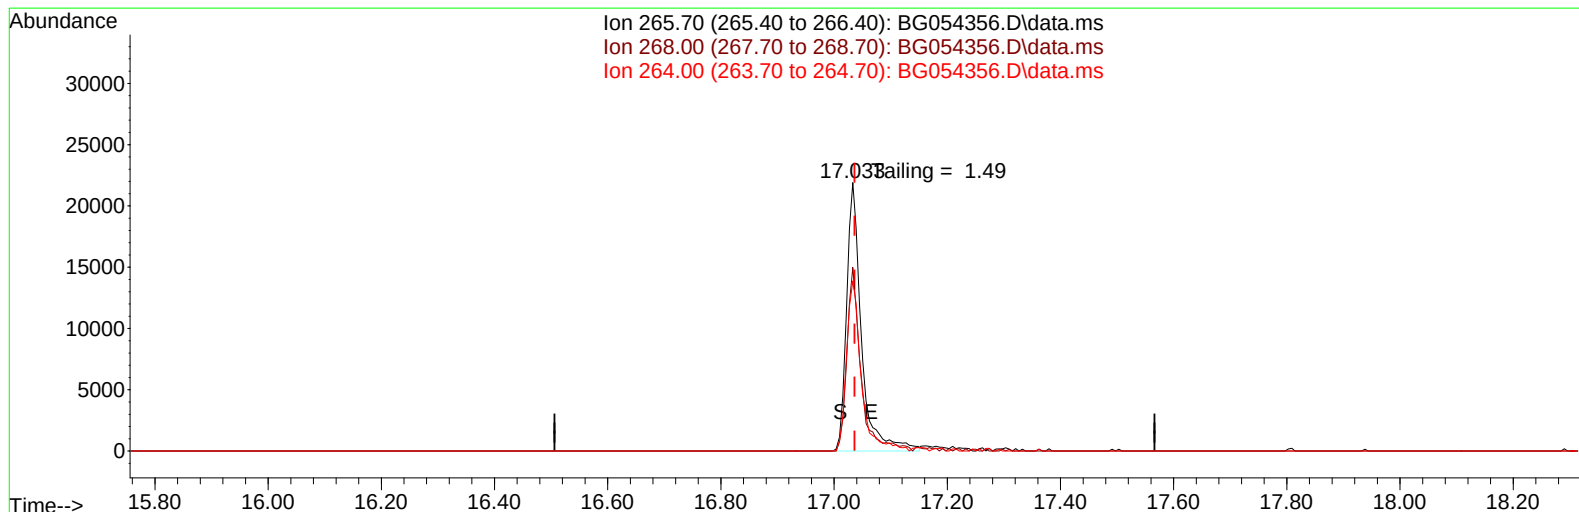

TIC: BG054356.D\data.ms

(70) Pentachlorophenol (C)




17.033min (-0.003) 27550.87 ng

response 40083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	72.43
264.00	66.20	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072222\
Data File : BG054356.D
Acq On : 22 Jul 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 02:06:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

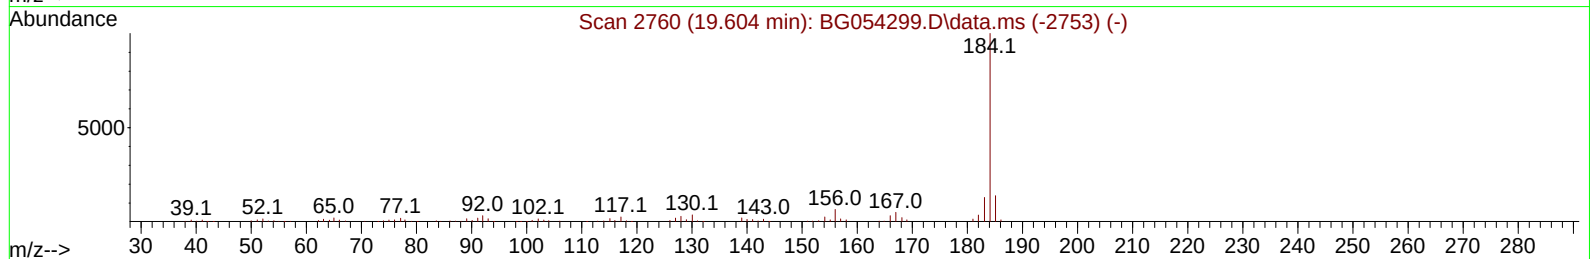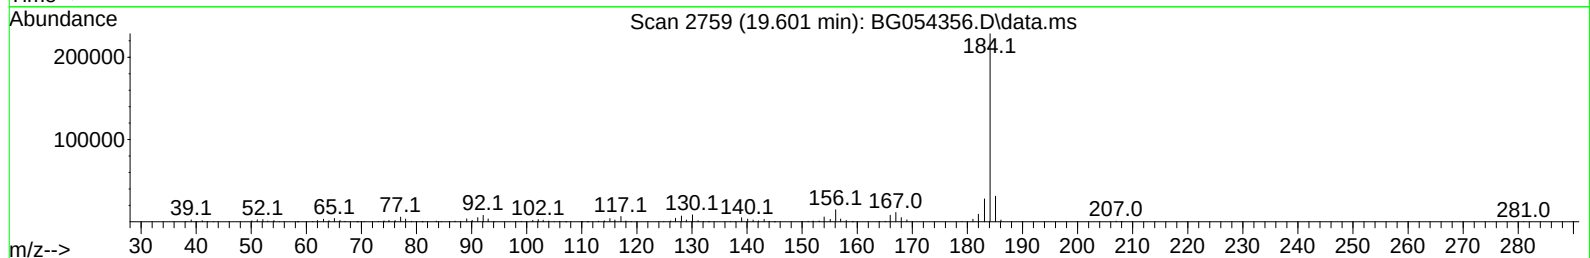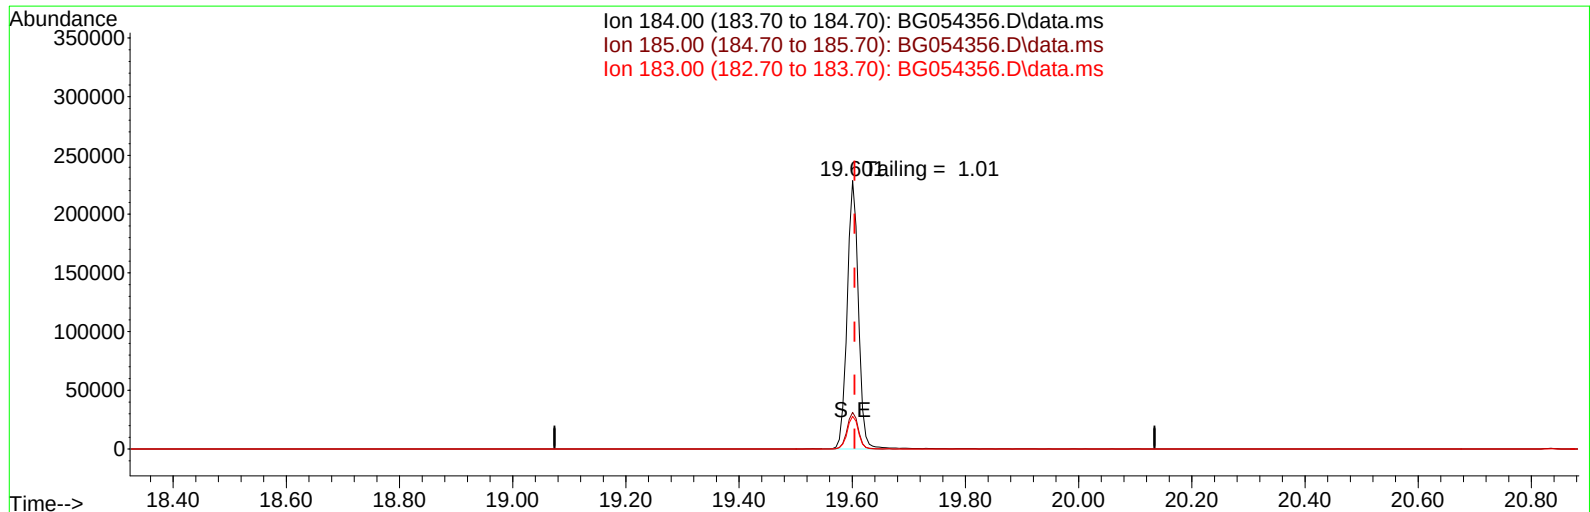

TIC: BG054356.D\data.ms

(77) Benzidine

19.601min (-0.003) 0.00 ng

response 314204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.70
183.00	11.10	12.19
0.00	0.00	0.00