
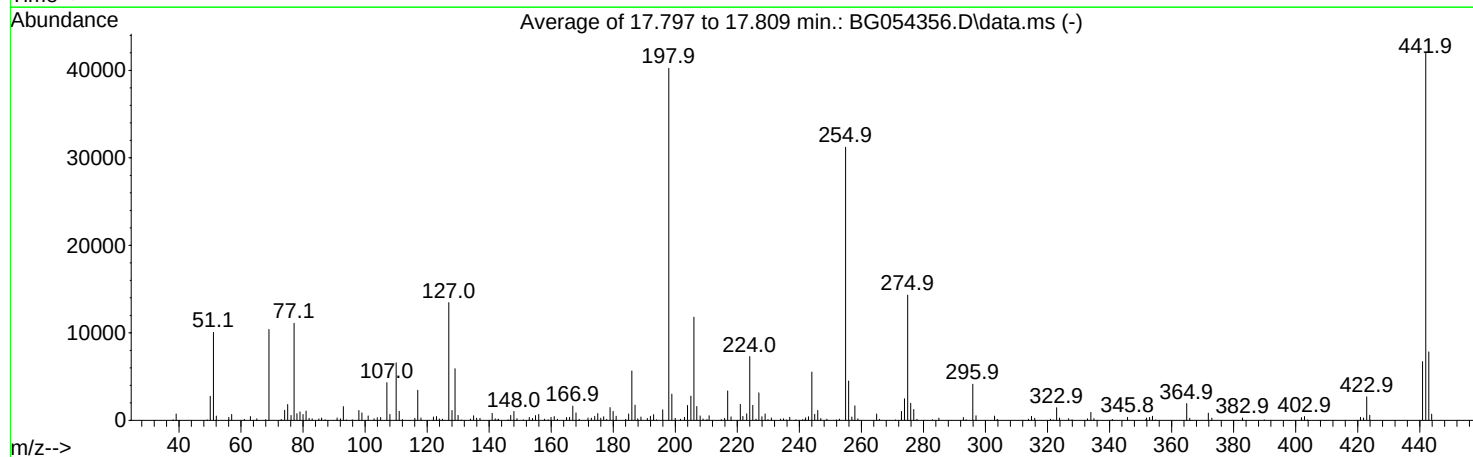


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072222\
 Data File : BG054356.D
 Acq On : 22 Jul 2022 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 15:54:11 2022

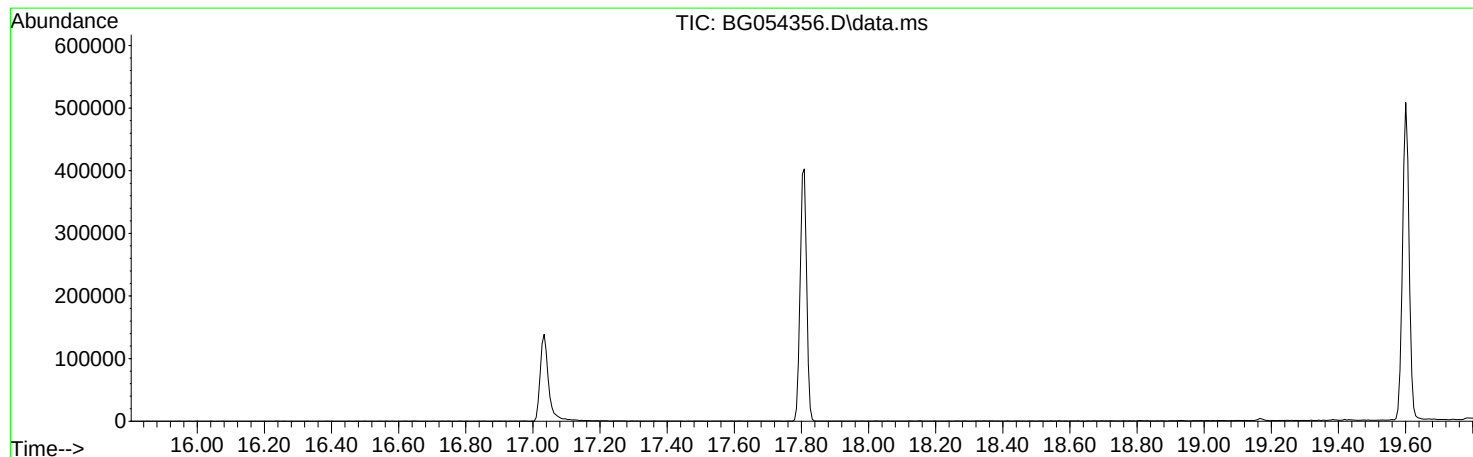




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	10060	PASS
68	69	0.00	2	0.7	73	PASS
69	198	0.00	100	25.8	10380	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.5	13468	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40235	PASS
199	198	5	9	7.4	2997	PASS
275	198	10	60	35.6	14313	PASS
365	198	1	100	4.8	1918	PASS
441	198	0.01	100	16.7	6713	PASS
442	442	50	100	100.0	42040	PASS
443	442	15	24	18.6	7818	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072222\
Data File : BG054356.D
Acq On : 22 Jul 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 02:06:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

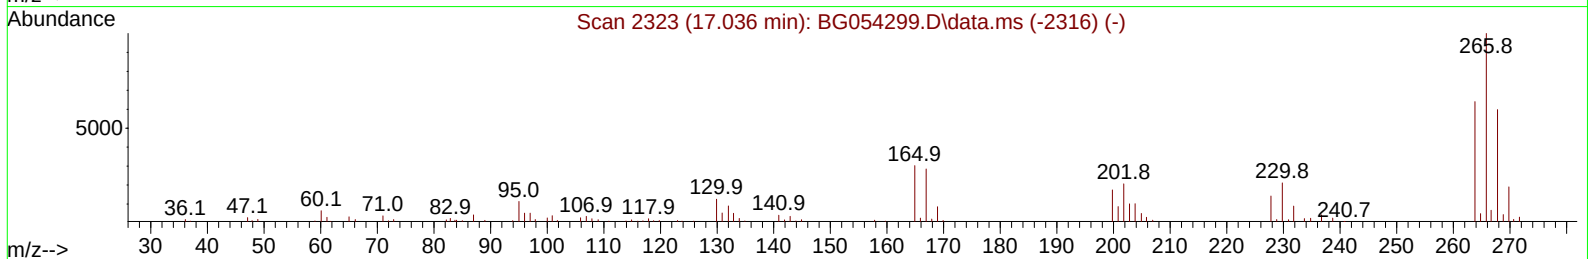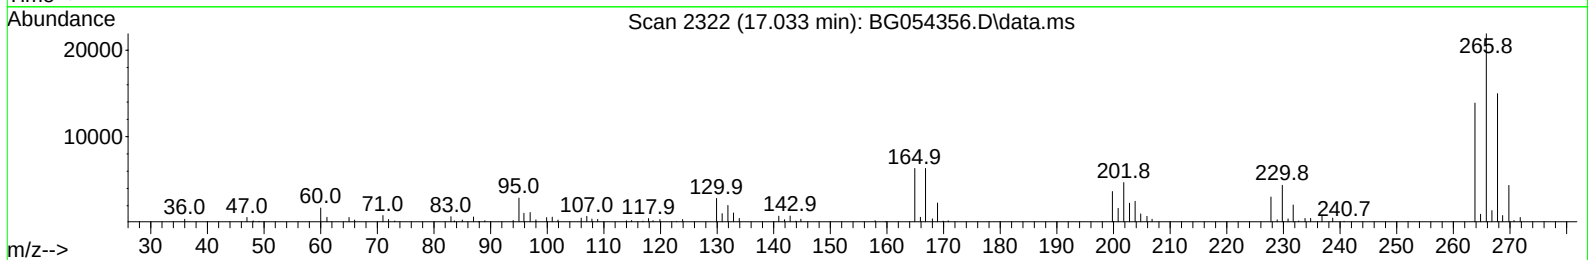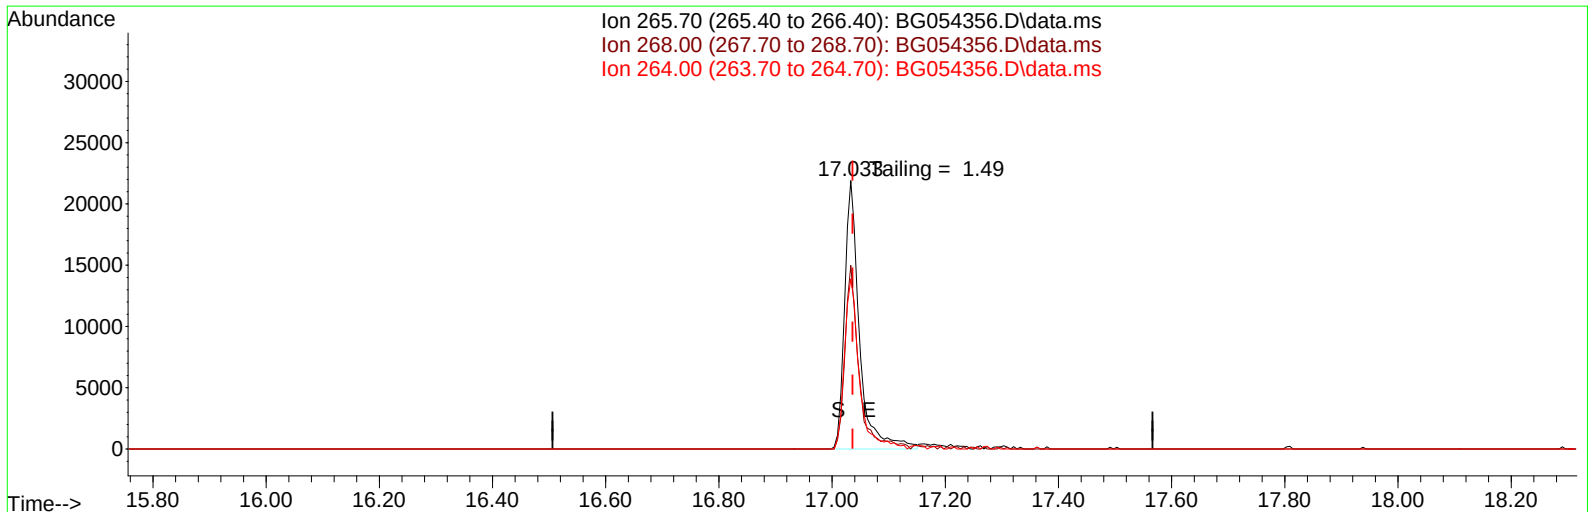

TIC: BG054356.D\data.ms

(70) Pentachlorophenol (C)

17.033min (-0.003) 27550.87 ng




response 40083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	72.43
264.00	66.20	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072222\
Data File : BG054356.D
Acq On : 22 Jul 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 23 02:06:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 15:54:11 2022
Response via : Initial Calibration

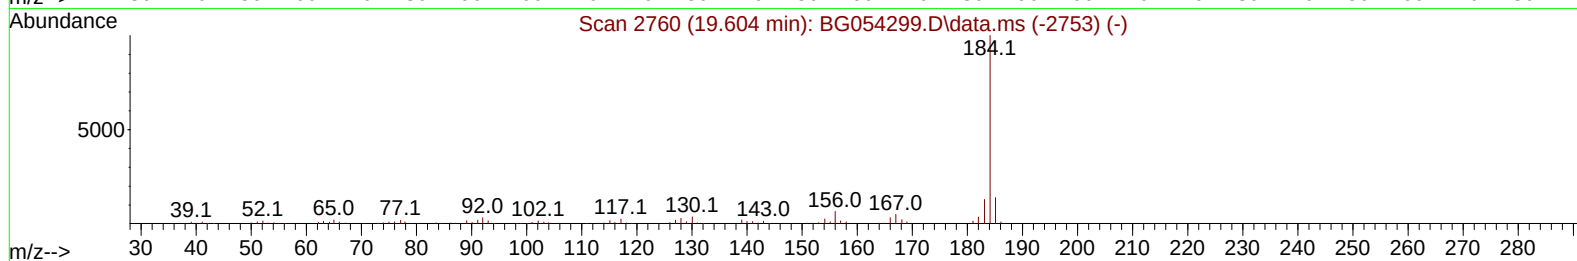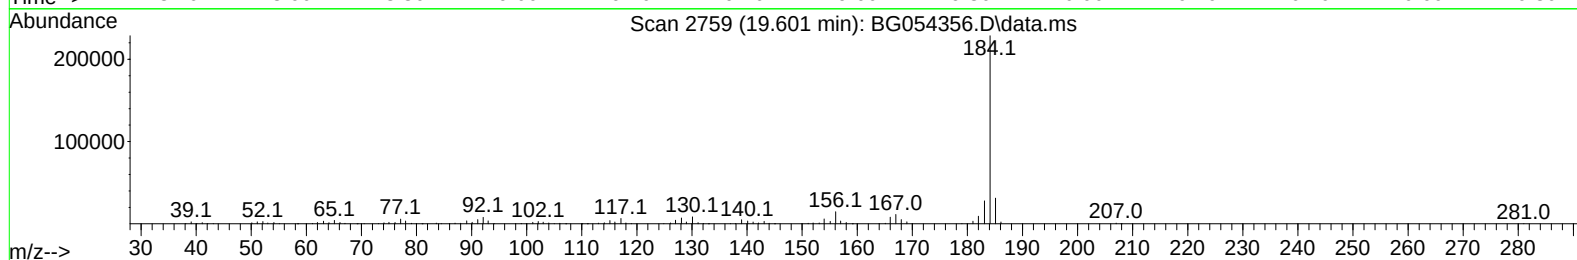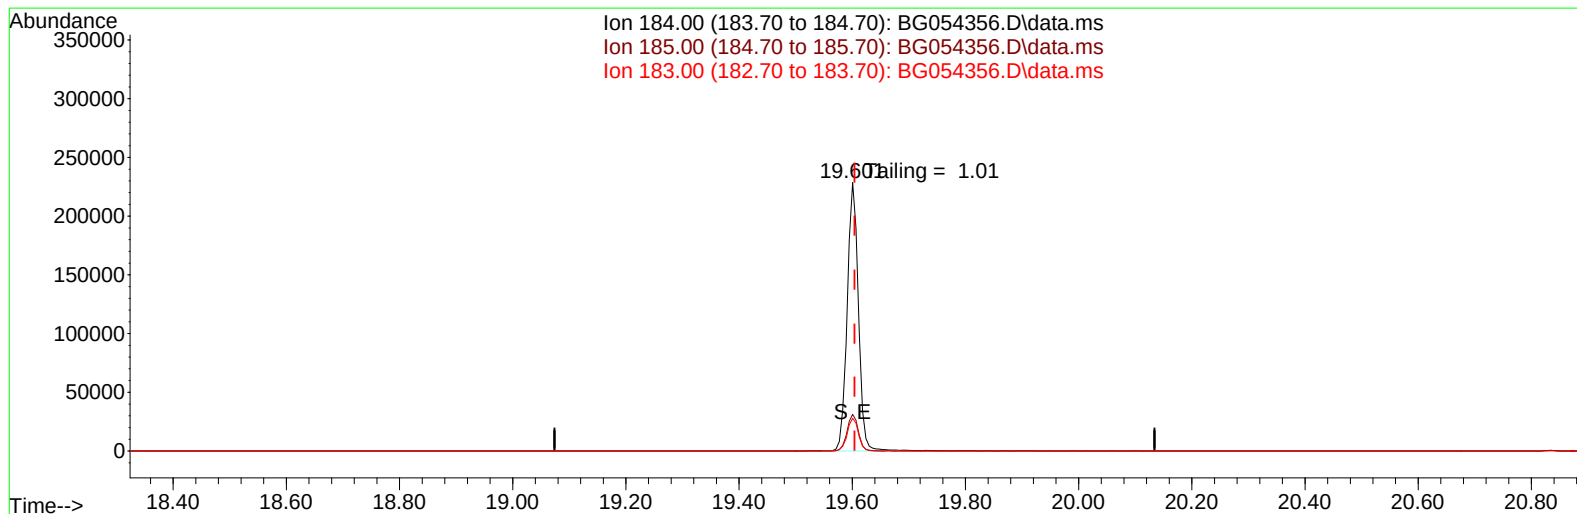

TIC: BG054356.D\data.ms

(77) Benzidine

19.601min (-0.003) 0.00 ng

response 314204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.70
183.00	11.10	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2022	BNA_G	<u>BG054356.D</u>
Compound Name	Response	Retention Time
DDT	173839	20.835
DDD	3024	20.394
DDE	77	19.889
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3101	176940	1.75

Instrument :
BNA_G
ClientSampleId :
DFTPP