

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072224\
 Data File : BG062165.D
 Acq On : 22 Jul 2024 17:34
 Operator : MA/JU
 Sample : PB162066BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	24	29	33	rBV4	14701	20456	1.09%	0.119%
2	3.669	64	65	68	rBV3	3315	2896	0.15%	0.017%
3	3.793	83	86	87	rBV2	3083	2683	0.14%	0.016%
4	3.875	96	100	111	rBV	178832	302220	16.05%	1.757%
5	4.016	122	124	127	rVB3	5067	4863	0.26%	0.028%
6	4.750	245	249	252	rBV4	1762	2653	0.14%	0.015%
7	5.162	316	319	323	rVB3	1685	2684	0.14%	0.016%
8	5.596	390	393	396	rBV2	1852	2703	0.14%	0.016%
9	6.319	511	516	518	rBV3	2177	3192	0.17%	0.019%
10	7.235	665	672	683	rBV	217643	379404	20.15%	2.206%
11	7.388	690	698	707	rVB	146456	244520	12.99%	1.422%
12	7.599	728	734	743	rVB	177633	324320	17.23%	1.886%
13	7.723	752	755	758	rVB	2452	2861	0.15%	0.017%
14	8.063	807	813	822	rBV2	154178	278253	14.78%	1.618%
15	8.780	928	935	943	rBV	260201	457899	24.32%	2.662%
16	9.232	1004	1012	1021	rBV	215562	375625	19.95%	2.184%
17	9.955	1127	1135	1143	rVB2	196037	353805	18.79%	2.057%
18	10.501	1221	1228	1239	rBV	288734	510107	27.10%	2.966%
19	10.877	1285	1292	1301	rVB	234958	418900	22.25%	2.435%
20	11.012	1307	1315	1322	rBV	261454	480565	25.53%	2.794%
21	12.446	1555	1559	1564	rBV3	5062	8074	0.43%	0.047%
22	12.569	1578	1580	1586	rBV	2391	3012	0.16%	0.018%
23	13.468	1729	1733	1738	rVB	1866	3734	0.20%	0.022%
24	14.091	1833	1839	1849	rVB	580631	807741	42.91%	4.696%
25	14.390	1879	1890	1898	rBV2	589287	907620	48.21%	5.277%
26	14.690	1934	1941	1950	rBV	434132	673568	35.78%	3.916%
27	14.913	1973	1979	1993	rBV	224825	387233	20.57%	2.251%
28	15.618	2093	2099	2103	rVB	2039	5014	0.27%	0.029%
29	15.683	2103	2110	2117	rBV	810660	1206156	64.07%	7.013%
30	15.806	2125	2131	2140	rBV	250600	390204	20.73%	2.269%
31	15.865	2140	2141	2144	rVB2	3901	2845	0.15%	0.017%
32	16.470	2239	2244	2247	rBV3	3425	6169	0.33%	0.036%
33	16.928	2320	2322	2324	rVB	2639	2763	0.15%	0.016%
34	17.081	2343	2348	2350	rVB	2192	3432	0.18%	0.020%
35	17.104	2350	2352	2357	rBV	2466	3922	0.21%	0.023%
36	17.233	2372	2374	2377	rBV	2180	2669	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072224\
 Data File : BG062165.D
 Acq On : 22 Jul 2024 17:34
 Operator : MA/JU
 Sample : PB162066BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
 Title : SVOA CALIBRATION

37	17.433	2402	2408	2416	rBV	623534	979654	52.04%	5.696%
38	17.533	2419	2425	2433	rVV	936182	1444299	76.72%	8.397%
39	17.656	2444	2446	2450	rVB2	2570	2754	0.15%	0.016%
40	17.762	2462	2464	2466	rBV	2752	2753	0.15%	0.016%
41	18.062	2511	2515	2516	rBV	2886	3099	0.16%	0.018%
42	18.091	2516	2520	2523	rVV3	3786	5766	0.31%	0.034%
43	18.138	2527	2528	2531	rVB2	4116	2955	0.16%	0.017%
44	18.702	2622	2624	2628	rBV	3962	4960	0.26%	0.029%
45	19.043	2679	2682	2685	rBV3	2298	2991	0.16%	0.017%
46	19.254	2717	2718	2721	rBV2	3704	4165	0.22%	0.024%
47	19.331	2730	2731	2735	rVB3	2997	3106	0.16%	0.018%
48	19.383	2735	2740	2745	rBV3	19238	31419	1.67%	0.183%
49	19.454	2747	2752	2756	rBV3	14995	23689	1.26%	0.138%
50	19.595	2775	2776	2779	rBV3	5235	5286	0.28%	0.031%
51	19.818	2808	2814	2820	rBV	1379298	1882481	100.00%	10.945%
52	21.698	3127	3134	3140	rBV2	712693	1208660	64.21%	7.027%
53	24.706	3636	3646	3656	rVB2	640622	1776448	94.37%	10.328%
54	24.923	3674	3683	3694	rVB2	419263	1230639	65.37%	7.155%




Sum of corrected areas: 17199889

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072224\
Data File : BG062165.D
Acq On : 22 Jul 2024 17:34
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

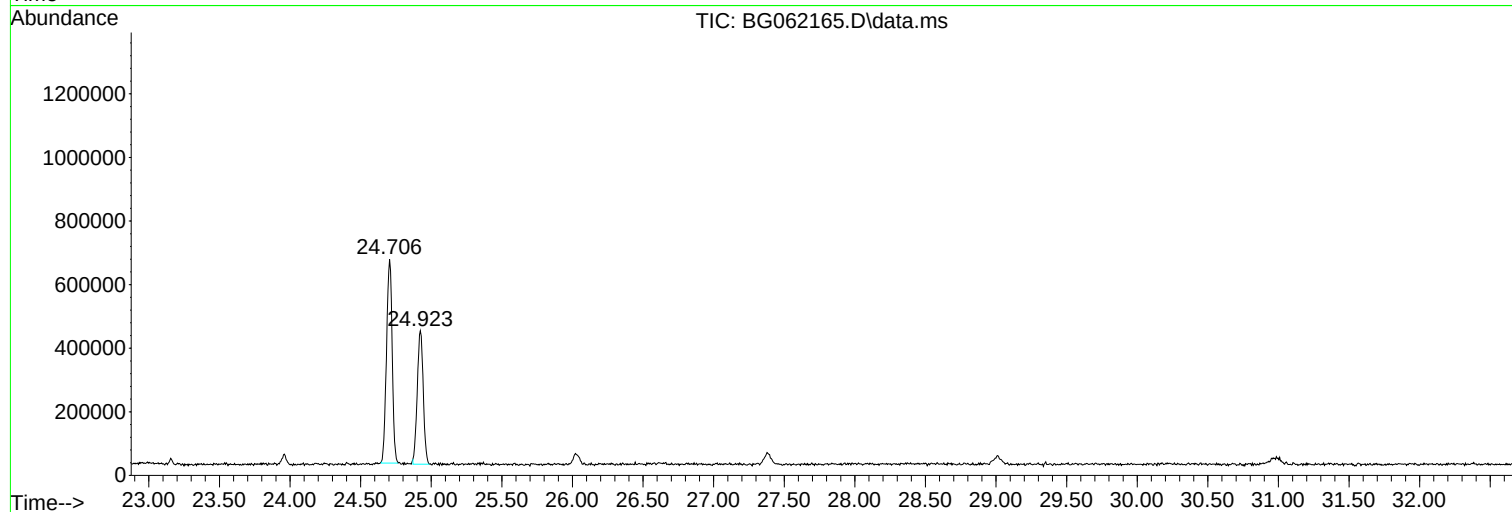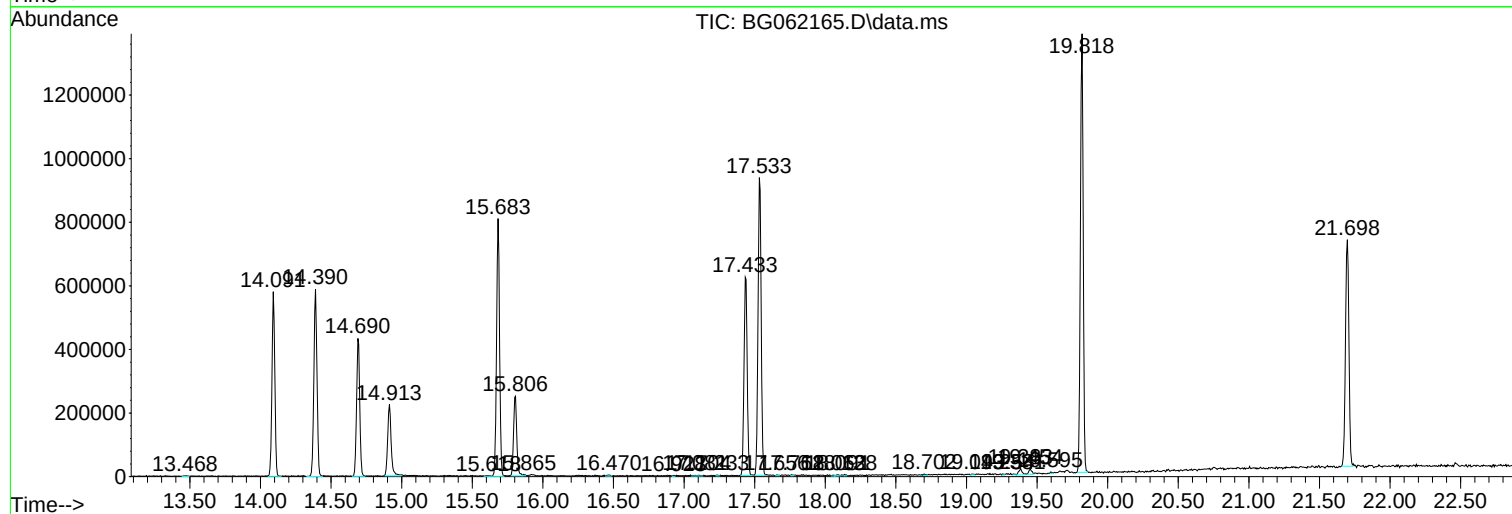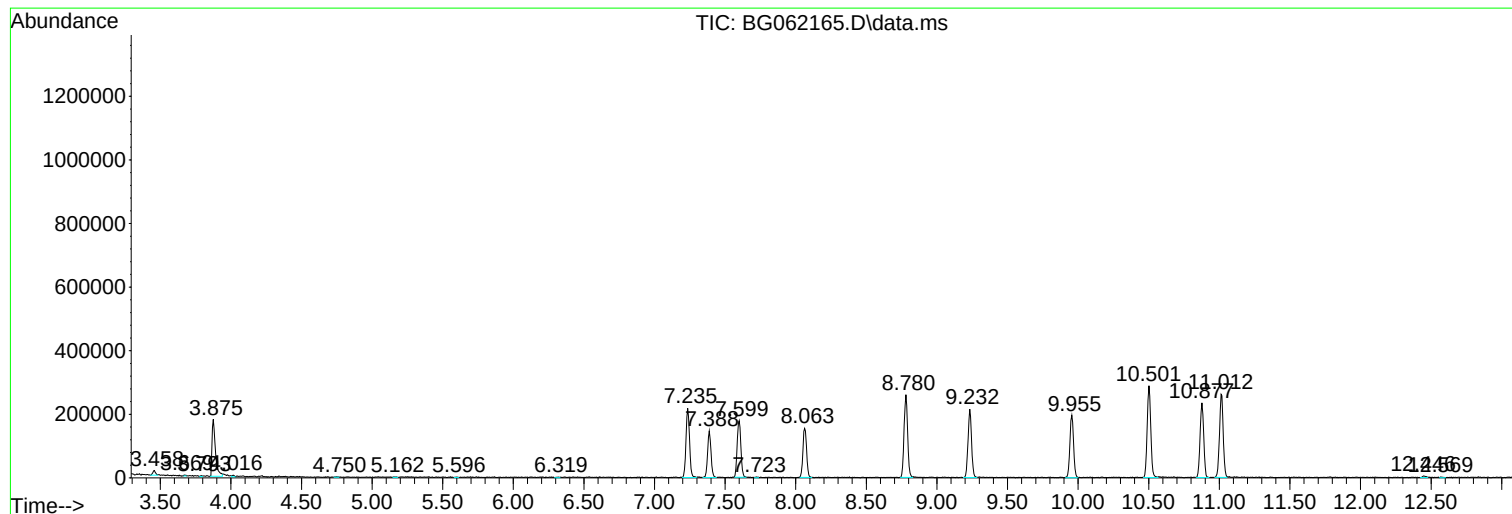

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072224\
Data File : BG062165.D
Acq On : 22 Jul 2024 17:34
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072224\
Data File : BG062165.D
Acq On : 22 Jul 2024 17:34
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------