

Data Path : Z:\HPCHEM1\BNA G\DATA\BG072315\
 Data File : BG018066.D
 Acq On : 23 Jul 2015 16:12
 Operator : TP/UM
 Sample : PB84595BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 24 01:07:20 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG072315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 23 16:20:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	47513	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	228437	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.18	164	153640	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.93	188	356180	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	378391	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	367231	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	7283	9.58	ng/uL	0.00
5) Phenol-d5	6.70	99	151873	41.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	84594	46.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	141775	43.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	139808	43.01	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	81434	45.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	88685	46.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	136380	41.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.44	131	220725	57.17	ng/ul	0.00
44) Dimethylphthalate-d6	13.60	166	509026	47.19	ng/ul	0.00
47) Acenaphthylene-d8	13.87	160	600973	45.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	101579	44.76	ng/ul	0.00
58) Fluorene-d10	15.18	176	453803	45.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	82510	36.23	ng/ul	0.00
71) Anthracene-d10	17.03	188	703171	45.58	ng/ul	0.00
79) Pyrene-d10	19.34	212	810148	46.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	815602	46.54	ng/ul	0.00

Target Compounds


					Ovalue
15) N-Nitroso-di-n-propylamine	8.23	70	3105	1.28 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG072315\
Data File : BG018066.D
Acq On : 23 Jul 2015 16:12
Operator : TP/UM
Sample : PB84595BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 24 01:07:20 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG072315.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 23 16:20:02 2015
Response via : Initial Calibration

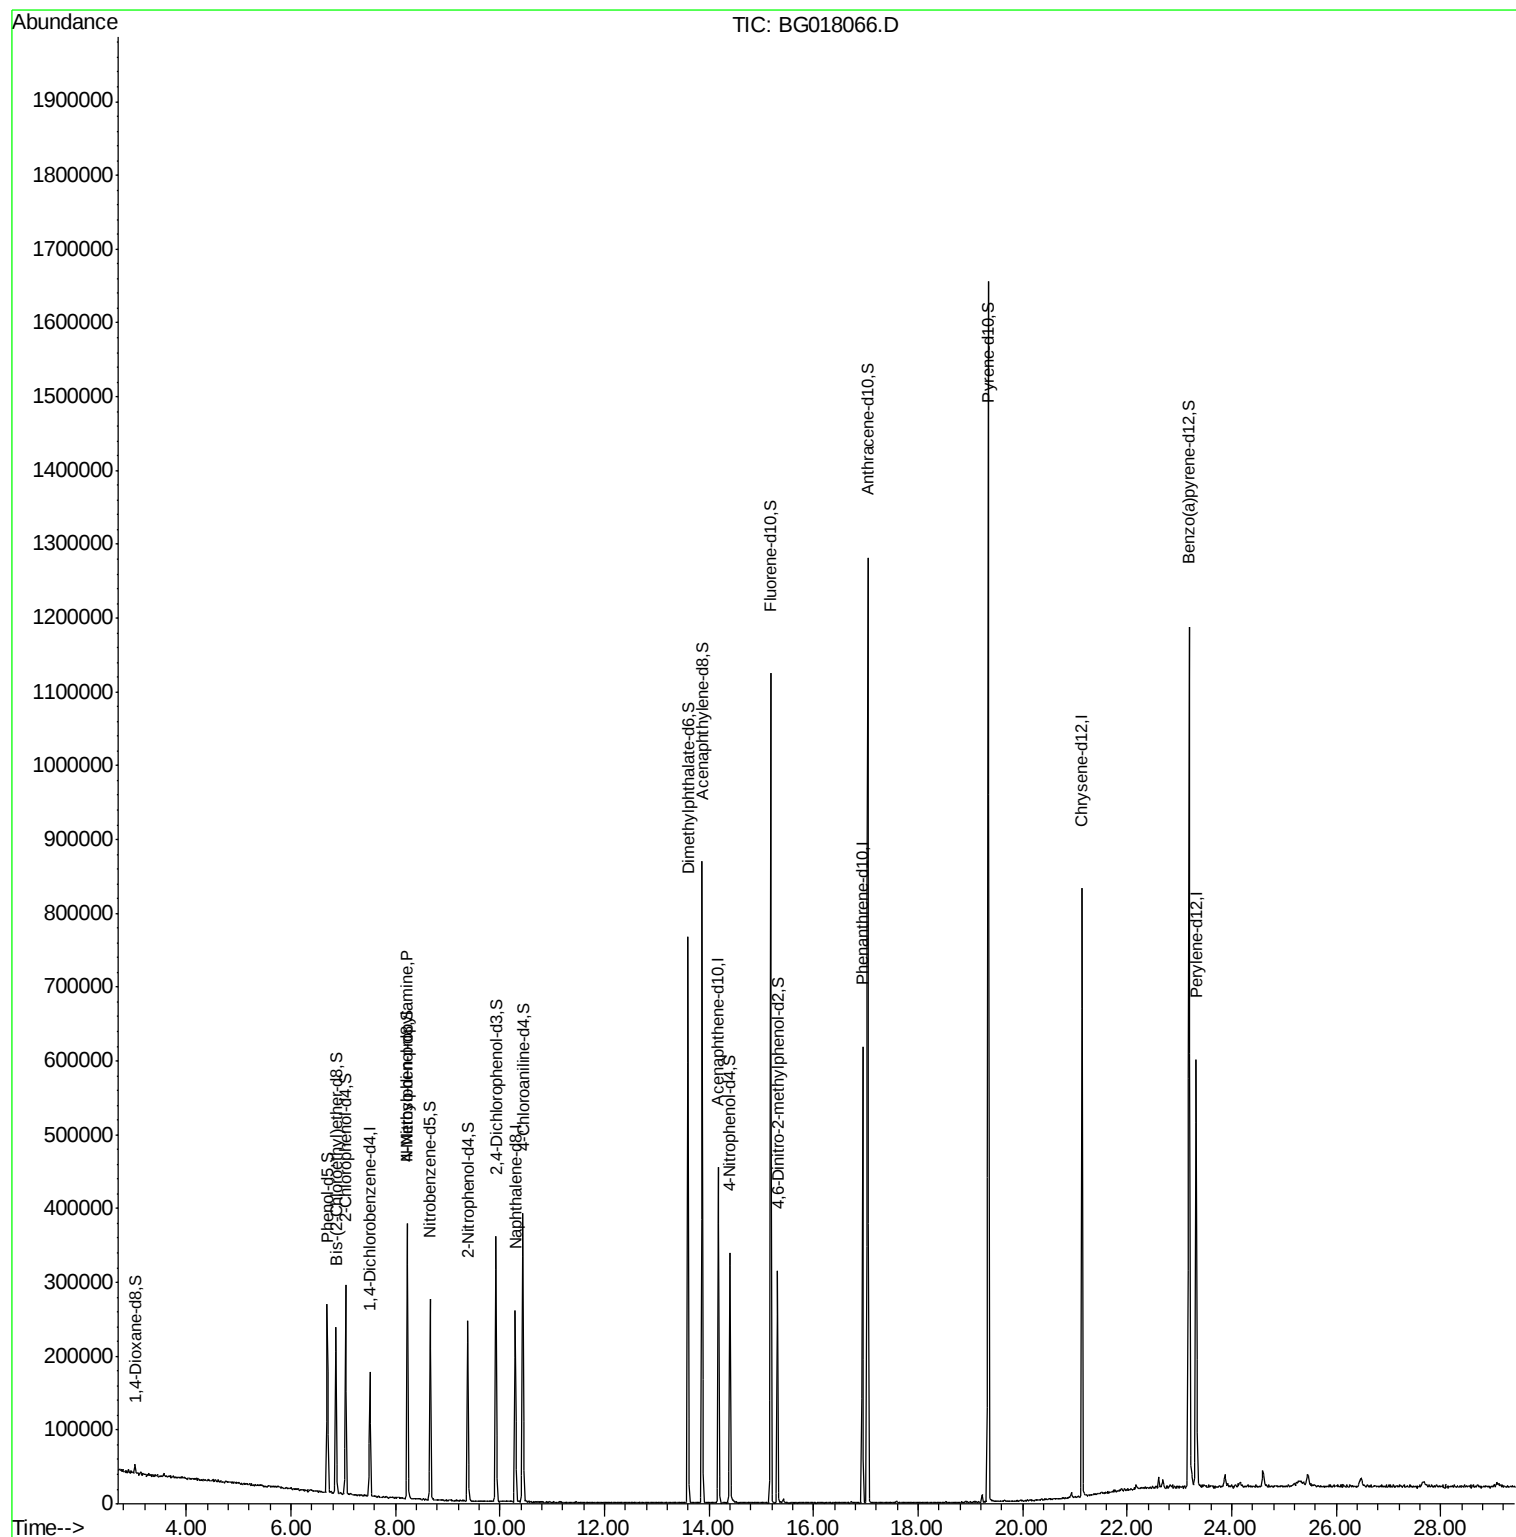

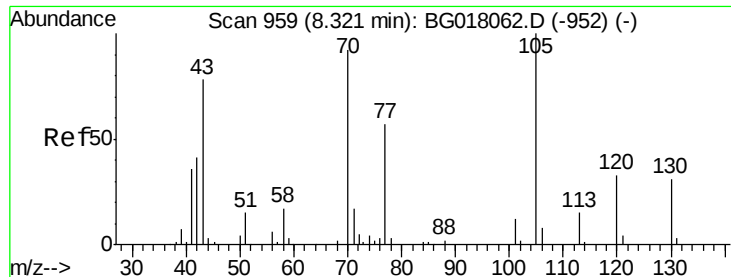

#15

N-Nitroso-di-n-propylamine

Concen: 1.28 ng/ul

RT: 8.23 min Scan# 944

Delta R.T. -0.09 min


Lab File: BG018066.D

Acq: 23 Jul 2015 16:12

Instrument :

BNA_G

ClientSampleId :

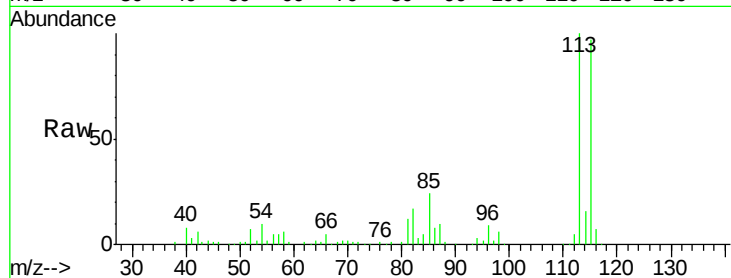

Tot Ion: 70 Resp: 3105


Ion Ratio Lower Upper

70 100

42 241.1 37.8 56.8#

101 0.0 10.0 15.0#

130 0.0 26.1 39.1#

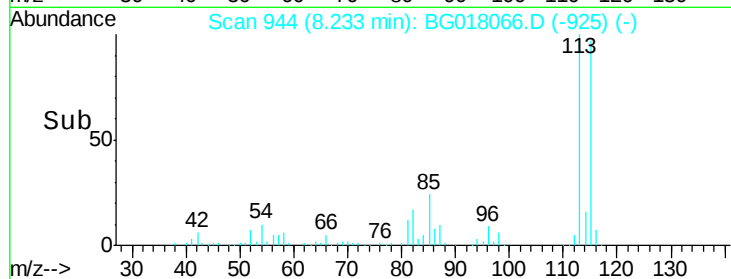

Abundance Ion 70.00 (69.70 to 70.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 101.00 (100.70 to 101.70): BGC

Ion 130.00 (129.70 to 130.70): BGC

